

# Composite of Poly Lactid Co-Glycolic Acid (PLGA)-Collagen Coated by Chitosan as Candidate of Hollow Fiber Small Diameter Vascular Graft

*by Prihartini Widiyanti*

---

**Submission date:** 13-May-2019 04:04PM (UTC+0800)

**Submission ID:** 1129596081

**File name:** C03\_Advanced\_Material\_Research\_2\_Okt\_2015.pdf (420.37K)

**Word count:** 2102

**Character count:** 11388

## Composite of Poly Lactid Co-Glycolic Acid (PLGA)-Collagen Coated by Chitosan as Candidate of Hollow Fiber Small Diameter Vascular Graft

Prihartini Widiyanti<sup>1,2,a</sup>, Dita Ayu Mayasari<sup>2,b</sup>, Zahrina Mardina<sup>2,c</sup>,

Riki Siswanto<sup>2</sup>, Agresta Afianti Ifada<sup>2</sup>, Ova Oktavina<sup>2</sup>

<sup>1</sup> Institute of Tropical Disease, Airlangga University, Surabaya, Indonesia

<sup>2</sup> Biomedical Engineering Program, Faculty of Science and Technology, Airlangga University, Surabaya, Indonesia

<sup>a</sup>drwidiyanti@yahoo.com, <sup>b</sup>mayasari.dita@gmail.com, <sup>c</sup>mardinazahrina@yahoo.com

**Keywords:** Chitosan, Collagen, PLGA, Hollow fiber, Vascular Graft

**Abstract.** Heart failure is a serious major health problem with high number of mortality per year. Bypass is one of solutions that has often been taken. Nowadays, synthetic materials have been fabricated from polymers to solve disadvantages which are provided by autograft, allograft and xenograft. The aim of this research is to make a synthetic vascular graft with great physical strength, high biocompatibility, and good affordability. The method of this research was mixing PLGA and collagen by magnetic stirrer. This composite were shaped by spinneret with water as coagulant. Then it was coated by chitosan with 3 variations of weight (1 %wt, 2 %wt, and 3 %wt) to increase hemo and cytocompatibility, proliferation, and cell attachment in order to make vascular graft candidates to be more biocompatible. Mechanical strength for each variation was 5,306 MPa (chitosan 1 %wt), 3,433 MPa (chitosan 2 %wt) and 3,745 MPa (chitosan 3 %wt). All tensile values were higher than human vascular tensile strength. Toxicity test showed that living cells in all variations were more than 60% in number, thus this vascular graft is not toxic. Hemolytic assay showed that the lowest coagulation was provided by sample with 3 %wt chitosan.

### Introduction

Heart failure is a major health problem. The prevalence of heart failure has tendency to be increased year by year. Most of patients diagnosed with heart failure still have around five years of life expectancy. There were approximately 250.000 patients died because heart failure each year, and that number has increased 6 times in last 40 years. The usage of natural materials or synthetic materials to replace part of a blood vessel in patient's recovery efforts has become very necessary [1].

The vascular graft which are made from pig aorta, bovine endothelial cell, rat cortex cerebral, or other xenograft materials (from another species) could hardly be developed in Indonesia due to several ethical problems and unsuitable societal paradigm. Stem cell development mainly the usage of non sterile medium such xenograft might cause zoonotic infection for human.

Even stem-cell-based medication of heart failure is believed to be future solution, this method is still unable to produce dramatic solving and cannot be practiced widely. One of reasons is the fact that only 0.5 – 5% of injected stem cells remain in targetted tissue while the rest just go through. Stem cell process is also very costly and time-consuming. In addition, there is also a problem to avoid contamination in laboratory. Moreover, when the product of stem cell is ready to be used, the cost which must be paid by the patient is very high. In contrary, there are more feasible procedures with other materials that could be done to minimize financial problem of heart failure and arteriosclerotic patients. Thus, a vascular graft made of synthetic polymers is developed. In the world, nowadays, polymers that have been used for vascular graft are PET, PTFE, Dacron, and several others. Each type of artificial vascular graft has advantages and disadvantages when viewed from its strength and biocompatibility. This study has been used Poly-L glycolic (PLGA). Lactid

glycolic acid compound itself tends to be not toxic because it is actually also a byproduct of metabolism. According to aforementioned backgrounds, an innovation of producing a vascular graft based on synthetic material Poly Lactid co Glycolic acid (PLGA) coated by chitosan in the form of micron hollow fiber was developed in this research. The purpose of using chitosan was to increase material's hemocompatibility and cytocompatibility, cell proliferation, and cell attachment. The PLGA was combined with bovine bone collagen to get a better modulus of elasticity that shown by ultimate tensile strength [2].

## Materials and method

### Materials

The materials used in this study were PLGA (Mw 100.000), DMF as solvent, bovine bone collagen, chitosan, acetic acid as solvent of chitosan, spinneret, and dip coating properties.

### Method

There were three process of creating hollow fiber PLGA. The first process was creating a homogenous solution. PLGA and bovine bone collagen were solved in DMF with concentration of 46%. Composition of solute was 76% PLGA and 24% bovine bone collagen. Solution was stirred without heating with velocity of radian 100 rpm for 5 hours. After that, solution was put in refrigerator for 24 hours. The second process was creating a hollow fiber with spinneret. The inert Nitrogen gasses were used to push solution out from syringe. The coagulant used in this process was water. The distance between the end of syringe and the coagulant bath was 2 cm. The result of spinneret can be seen on figure 1.

The third process was coating hollow fiber with chitosan. There were three variation of chitosan concentration 1%wt, 2%wt, and 3%wt. Chitosan was dissolved in acetic acid. Then, the hollow fiber was dipped in chitosan solution for 2 hours and dried with oven in temperature of 40° C for 24 hours.



Fig 1. Hollow fiber PLGA-bovine bone collagens

The fourth process was mechanical, biological, chemical and physical characterization. Mechanical characterization was tensile strength test with autograph. Cytotoxicity test as biological characterization used MTT Assay. The physical characterization was microscopy test used scanning electron micrograph and chemical characterization was hemocompatibility test used hemolysis method.

## Results

### Ultimate Tensile Strength

The mechanical properties evaluations were done to acquire the values of hollow fiber's mechanical quality. A tensile strength test was done with two repetitions.

Table 1. Result of Tensile Strength Test

Sample (concentration of chitosan)	Ultimate Tensile Strength (MPa)
1 %wt	5.306
2 %wt	3.433
3 %wt	3.745

The extension rate of autograph used in this research was 5 mm/minute. The average diameter of hollow fiber sample tested in autograph was 2 mm.

### Cytotoxicity Test

The second evaluation was cytotoxicity test using Baby Hamster Kidney cell 21 (BHK 21) by MTT assay method.

Table 2. MTT Assay Result

Sample (concentration of chitosan)	OD Media Control	OD Cell Control	OD Sample	% Live Cell
1 %wt	0.129	0.125	0.117	95.7
2 %wt	0.130	0.124	0.105	92.5
3 %wt	0.126	0.120	0.110	95.7

### Morphological

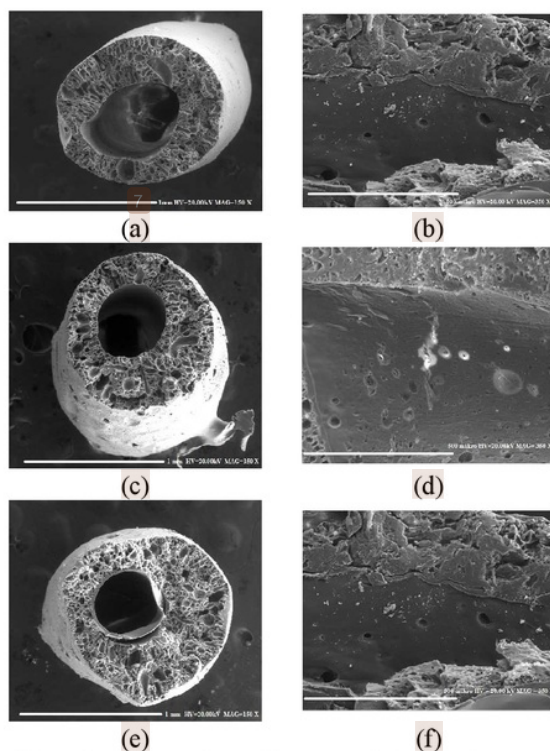


Fig 2. Hollow fiber PLGA-collagen coating chitosan 1 %wt with magnification 100× (a), inner surface of hollow fiber PLGA-collagen coating chitosan 1 %wt with magnification 350× (b), Hollow fiber PLGA-collagen coating chitosan 2 %wt with magnification 150× (c), inner surface of hollow fiber PLGA-collagen coating chitosan 2 %wt with magnification 350× (d), Hollow fiber PLGA-collagen coating chitosan 3 %wt with magnification 150× (e), inner surface of hollow fiber PLGA-collagen coating chitosan 3 %wt with magnification 350× (f)



### Hemolytic Test

For hemolysis test, the percentage of coagulation was calculated by using Eq. 1 :

$$\%D = \frac{A_{sample} - A_{negatif}}{A_{positif} - A_{negatif}} \times 100\% \quad (\text{Equation 1})$$

Table 3. Hemolysis Result

Sampel (Concentration of Chitosan)	%D (%)
1 %wt	63.8
2 %wt	15
3 %wt	8.3

### Discussion

#### Ultimate Tensile Test

From Table 1, it was shown that the lowest chitosan concentration (1 %wt) had highest ultimate tensile strength (5.306 Mpa) while the value for 2% and 3% were almost similar. This phenomenon might be caused by an increased rate of chitosan infiltration through nanofiber pores due to smaller concentration. Thus, the mechanical strength was increased. The increase of tensile strength was also attributed to the stronger interfacial adhesion between polymer and coater [3].

#### Citotoxicity Test

A material is toxic if the value of optical density was less than 60%. The result of living cell percentage of samples were more than 60% and it could be concluded that material was a nontoxic material [4].

#### Morphological Analysis

Based on SEM characterization, the thickness of sample with coating 1 %wt was 0,3µm and the porous was 41,32 µm. The thickness of sample with coating 2 %wt was 0,4µm and the porous was 79,76µm. The thickness of sample with 3 %wt of coating was 0,49µm and the pores were 108,95µm in diameter. A big number of pores showed that the infiltration of chitosan particle was low due to its high solution viscosity. In contrary, small number of pores showed high density of chitosan particles in the hollow fiber that caused a higher ultimate strength [5].

#### Hemolytic Test

High percentage of coagulation showed that there were many thromboses [6]. Thrombosis can be prevented by making the inner surface of hollow fiber smoother [6]. Since the inner surface of sample with 3 %wt of chitosan was thicker, the thrombosis can be inhibited [7].

### Conclusion

1. The highest tensile strength is provided by sample with 1 %wt chitosan caused by an increased rate of chitosan infiltration through nanofiber pores due to smaller concentration
2. The result of living cell percentage of samples are more than 60% and it could be concluded that the material is a nontoxic material
3. High chitosan concentration provides a big number of pores because the infiltration of chitosan particle is low due to its high solution viscosity. In contrary, Low chitosan concentration provides a small number of pores due to better infiltration of particle and it causes a higher ultimate tensile strength
4. Sample with highest chitosan concentration provides the lowest coagulation because thick concentration of chitosan makes inner surface of vascular graft smoother.

### Acknowledgements

Our great gratitude is delivered to Directorate of Higher Education (DIKTI) Ministry of National Education for funding through student creativity program. This investigation and the paper were supported in part, by Mrs. Siti Wafiroh, Ms. Vita, Ms. Mahdiya Nayla, Ms. Azisya AK and all the parties involved in the completion of this paper.

### References

- [1] Roger VL, Go AS, Lloyd-Jones DM, Benjamin EJ, Berry JD, Borden WB, et al. Heart disease and stroke statistics. 2012 update: a report from the American Heart Association. *Circulation*. 2012;125(1):e2–220.
- [2] Kim, Mi Jin. et. al. In vitro and in vivo Application of PLGA Nanofiber for Artificial Blood Vessel. *Macromolecular Research*, Vol. 16, No. 4, pp 345-352 (2008)
- [3] Polymer society, Polymer nanocomposites. Woodhead publishing and Maney publishing. Boston, New York.
- [4] Spielmann, H., et al. The ECVAM International Validation Study on In Vitro Tests for Acute Skin Irritation: Report on the Validity of the EPISKIN and EpiDerm Assays and on the Skin Integrity Function Test. *ATLA* 35, 559-601, 2007
- [5] Chawla, N and Deng, X. Effect of density in the microstructure and the mechanical behavior of powder metallurgy Fe-Mu-Ni steels. *Mechanical Behavior of Materials Facility, Arizona State University*
- [6] Vijayanand, K.; Deepak, K.; Pattanayak, D.K.; Rama Mohan, T.R. & Banerjee, R. (2005). Interpreting Blood-Biomaterial Interactions from Surface Free Energy and Work of Adhesion. *Trends in Biomaterials and Artificial Organs*, Vol.18, No.2, (January 2005), pp. 73-83, ISSN 0971-1198
- [7] Fink, H., et al. 2011. An in vitro study of blood compatibility of vascular grafts made of bacterial cellulose in comparison with conventionally-used graft materials. *Journal of Biomedical Materials Research Part A*, 97A, 52-58.

**Materials, Industrial, and Manufacturing Engineering Research Advances 2**

10.4028/www.scientific.net/AMR.1125

**Composite of Poly Lactid Co-Glycolic Acid (PLGA)-Collagen Coated by Chitosan as Candidate of Hollow Fiber Small Diameter Vascular Graft**

10.4028/www.scientific.net/AMR.1125.411

**DOI References**

[2] Kim, Mi Jin. et. al. In vitro and in vivo Application of PLGA Nanofiber for Artificial Blood Vessel.

Macromolecular Research, Vol. 16, No. 4, pp.345-352 (2008).

10.1007/bf03218527

[3] Polymer society, Polymer nanocomposites. Woodhead publishing and Maney publishing. Boston, New York.

10.1016/b978-0-85709-777-4.50020-6

[7] Fink, H., et al. 2011. An in vitro study of blood compatibility of vascular grafts made of bacterial cellulose in comparison with conventionally-used graft materials. Journal of Biomedical Materials Research Part A,

97A, 52-58.

10.1002/jbm.a.33031

# Composite of Poly Lactid Co-Glycolic Acid (PLGA)-Collagen Coated by Chitosan as Candidate of Hollow Fiber Small Diameter Vascular Graft

## ORIGINALITY REPORT

8%

SIMILARITY INDEX

6%

INTERNET SOURCES

7%

PUBLICATIONS

0%

STUDENT PAPERS

## PRIMARY SOURCES

1

[citeseerx.ist.psu.edu](https://citeseerx.ist.psu.edu)

Internet Source

2%

2

[itd.unair.ac.id](http://itd.unair.ac.id)

Internet Source

2%

3

Aunbamrung, Pornthip, and Akkarat Wongkaew. "Effect of Calcination Temperatures of Cu/CeO<sub>2</sub>-Containing Co on Physiochemical Properties and Catalytic Activity to Selective CO Oxidation", *Advanced Materials Research*, 2015.

Publication

2%

4

[www.portalgaruda.org](http://www.portalgaruda.org)

Internet Source

1%

5

Ananoria, A., and Bryan Pajarito. "Effect of Ingredient Loading on Water Transport Properties of a Vulcanized Natural Rubber Compound", *Advanced Materials Research*, 2015.

1%



6

Baharuddin, Baharuddin, Suhariningsih  
Suhariningsih, and Brodjol Sutijo Suprih Ulama.  
"Geographically Weighted Regression Modeling  
for Analyzing Spatial Heterogeneity on  
Relationship between Dengue Hemorrhagic  
Fever Incidence and Rainfall in Surabaya,  
Indonesia", Modern Applied Science, 2014.

Publication

<1%

7

library.umac.mo

Internet Source

<1%

---

Exclude quotes      Off

Exclude matches      < 7 words

Exclude bibliography      On

# Composite of Poly Lactid Co-Glycolic Acid (PLGA)-Collagen Coated by Chitosan as Candidate of Hollow Fiber Small Diameter Vascular Graft

---

## GRADEMARK REPORT

---

FINAL GRADE

**/0**

GENERAL COMMENTS

**Instructor**

---

PAGE 1

---

PAGE 2

---

PAGE 3

---

PAGE 4

---

PAGE 5

---

PAGE 6

---