

username:
password:

Optoelectronics and Advanced Materials - Rapid Communications (OAM-RC)

[Home](#) [Editorial information](#) [Reviewing Procedure](#) [Electronic Journals](#) [Manuscript submission](#)
[Browse Volumes](#) [Subscription](#) [Copyright Transfer](#) [Board](#) [Contact](#)

SITE NEWS

Online Papers
Optoelectronics and Advanced Materials-Rapid Communications (OAM-RC) offers now the possibility to read the papers on-line. Starting with the Issue 1, Volume 1, 2007 you can bring the full papers of OAM-RC on your computer.

JOAM
Journal of Optoelectronics and Advanced Materials

INOE Publishing House
Integra Natura Omnia et Aeterna

TOP VIEWED ARTICLES

- » Van der Waals three-body force shell model (VTSM) for the Lattice dynamical studies of Potassium fluoride (14804)
- » Effect of Aluminum mole fraction and well width on the probability density spreading in GaN/AlGaIn quantum well (7562)
- » Highly conducting and transparent multilayer films based on ZnO and Mo-doped indium oxide for optoelectronic applications (4097)

STATISTICS

Last update: 2017-12-08
Visitors: 2785673

Welcome to our website!

JOURNAL SCOPE

The **Optoelectronics and Advanced Materials - Rapid Communications (Optoelectron. Adv. Mat.)** appears with 12 issues per year. It is an associated letter journal to Journal of Optoelectronics and Advanced Materials. Optoelectron. Adv. Mat. is dedicated to the rapid publication of short papers and, in particular, breaking news in the field of optoelectronics, photonics, and new advanced materials (nonlinear optical materials, crystalline and non-crystalline materials, nano-structured materials, functional and smart materials, materials based on polymers, biomaterials) of relevance for optoelectronics and photonics.

Optoelectronics and Advanced Materials-Rapid Communications has been accepted for the following Thomson ISI products beginning with volume 1(1) 2007:

Science Citation Index-Expanded (SCIE) including the *Web of Science*

ISI Alerting Service

Materials Science Citation Index (MSCI)

Print: ISSN 1842-6573

On-line: ISSN 2065-3824

Manuscripts should be sent to the following e-mail:

oam-rc@inoe.ro

For any other information please contact us at:

journals@inoe.ro

FAST PUBLICATION TAX

For authors who want a fast publication in our journals, the new tax, starting from January 22, 2015 is in amount of 300 Euros (350 USD, 1400 RON). Authors will be invoiced and the proforma invoice will be sent via e-mail, after the reviewing and the approval of the paper. Please, inform us during the submission of the paper.

Journal Impact Factor (2016): 0.470 - 2016 Journal Citation Reports (Clarivate Analytics, 2017)

username:
password:

Optoelectronics and Advanced Materials - Rapid Communications (OAM-RC)

[Home](#) [Editorial information](#) [Reviewing Procedure](#) [Electronic Journals](#) [Manuscript submission](#)
[Browse Volumes](#) [Subscription](#) [Copyright Transfer](#) [Board](#) [Contact](#)

SITE NEWS

Online Papers
Optoelectronics and Advanced Materials-Rapid Communications (OAM-RC) offers now the possibility to read the papers on-line. Starting with the Issue 1, Volume 1, 2007 you can bring the full papers of OAM-RC on your computer.

JOAM
Journal of Optoelectronics and Advanced Materials

INOE Publishing House
Integra Natura Omnia et Aeterna

TOP VIEWED ARTICLES

- » Van der Waals three-body force shell model (VTSM) for the Lattice dynamical studies of Potassium fluoride (14804)
- » Effect of Aluminum mole fraction and well width on the probability density spreading in GaN/AlGaIn quantum well (7582)
- » Highly conducting and transparent multilayer films based on ZnO and Mo-doped indium oxide for optoelectronic applications (4097)

STATISTICS

Last update: 2017-12-08
Visitors: 2786079

Board

EDITOR-IN-CHIEF

ADRIAN PETRIS

National Institute for Laser, Plasma and Radiation Physics, Magurele-Ilfov, Romania

DIRECTOR OF PUBLICATION

ROXANA SAVASTRU

National Institute for Optoelectronics, Magurele-Ilfov, Romania

DEPUTY DIRECTOR OF PUBLICATION

Roxana Radvan

National Institute of Optoelectronics, Magurele-Ilfov, Romania

EDITORIAL BOARD:

PETER B. BARNA – *Research Institute for Technical Physics and Materials Science, Budapest, Hungary*

EMIL BURZO – *Babes-Bolyai University, Cluj-Napoca, Romania*

GERALD LUCOVSKY – *North-Caroline State University, Raleigh, USA*

MICHAEL PAESLER – *North-Caroline State University, Raleigh, USA*

JAMES C. PHILLIPS – *Rutgers University, Piscataway, USA*

BOUCHTA SAHRAOUI – *University of Angers, France*

JAI SINGH – *Charles Darwin University, Darwin, Australia*

VALENTIN VLAD – *Romanian Academy; National Institute for Laser, Plasma and Radiation Physics, Măgurele-Ilfov, Romania*

ADVISORY BOARD:

ADRIAN BETERINGHE – *Institute of Physical Chemistry "Ilie Murgulescu", Bucharest, Romania*

HORIA CHIRIAC – *National Institute of Research & Development for Technical Physics, Iasi, Romania*

MIKHAIL F. CHURBANOV – *Institute of Chemistry of High-Purity Substances of the Academy of Sciences, Nizhny Novgorod, Russia*

GHEORGHE CIOBANU – *University of Bucharest, Romania*

MAGDALENA L. CIUREA – *National Institute of Materials Physics, Măgurele-Ilfov, Romania*

PETER J. S. EWEN – *School of Engineering and Electronics, Edinburgh, UK*

WILHELM KAPPEL – *Research and Design Institute for Electrotechnics, Bucharest, Romania*

ALEXANDRU LUPASCU – *"Politehnica" University, Bucharest, Romania*

VIKTOR S. MINAEV – *Research Institute of Material Science and Technology, Moscow, Russia*

ZHIHUA XU – *Brookhaven National Laboratory, USA*

DIANA NESHEVA – *Institute of Solid State Physics, Sofia, Bulgaria*

STAVROS PISSADAKIS – *FORTH-IESL, Heraklion, Greece*

ADRIAN PODOLEANU – *University of Kent, Canterbury, UK*

K. S. SANGUNNI – *Indian Institute of Science, Bangalore, India*

TOMAS WAGNER – *University of Pardubice, Pardubice, Czech Republic*

ZHENG-MAO WU – *Southwest University, Changqing, China*

ATHANASIE TRUTIA – *University of Bucharest, Romania*

MARIA ZAHARESCU – *Institute of Physical Chemistry "Ilie Murgulescu", Bucharest, Romania*

JAN ZAVADIL – *Institute of Photonics and Electronics, Academy of Sciences, Prague, Czech Republic*

XIANG-HUA ZHANG – *University of Rennes, Rennes, France*

PUBLISHING BOARD

Teodorina Victoria Belegante

Monica Mariana Vlad

Mihaela Alina Dragan

PRODUCTION AND HANDLING

Maria Nedelcu

username:
password:
Go

Optoelectronics and Advanced Materials - Rapid Communications (OAM-RC)

[Home](#) [Editorial information](#) [Reviewing Procedure](#) [Electronic Journals](#) [Manuscript submission](#)
[Browse Volumes](#) [Subscription](#) [Copyright Transfer](#) [Board](#) [Contact](#)

SITE NEWS

Online Papers

Optoelectronics and Advanced Materials-Rapid Communications (OAM-RC) offers now the possibility to read the papers on-line. Starting with the Issue 1, Volume 1, 2007 you can bring the full papers of OAM-RC on your computer.

JOAM

Journal of Optoelectronics and Advanced Materials

INOE Publishing House

Integra Natura Omnia et Aeterna

TOP VIEWED ARTICLES

- » Van der Waals three-body force shell model (VTSM) for the Lattice dynamical studies of Potassium fluoride (14604)
- » Effect of Aluminum mole fraction and well width on the probability density spreading in GaN/AlGaIn quantum well (7582)
- » Highly conducting and transparent multilayer films based on ZnO and Mo-doped indium oxide for optoelectronic applications (4097)

STATISTICS

Last update: 2017-12-08
Visitors: 2785977

High repetition rate graphene passively Q-switched YVO4/Nd:YVO4 laser

Author: J. W. ZHANG, M. B. LI, N. ZHANG, K. X. LI, W. Z. JIANG

Viewed 69 times

A passively Q-switched Yb3+-doped all-fiber laser based on SBS effect

Author: LIAN-JU SHANG, ZHEN-ZHONG CAO, XIU-QIN YANG

Viewed 53 times

EDFA gain flattening using cascaded fiber Bragg gratings

Author: DALIA SALLAM, ISLAM ASHRY, ALI ELRASHIDI, ZIAD A. EL-SAHN, MOUSTAFA H. ALY

Viewed 41 times

Binary optimization of plasmonic nano-disk-based absorption coefficient

Author: MILAD KABOLI, MAJID AKHLAGHI, MOHSEN BALVASI, HOSSEIN SHAHMIRZAE

Viewed 45 times

Thirring optical solitons in birefringent fibers with parabolic law nonlinearity

Author: ALI SARDAR, SYED TAHIR RAZA RIZVI, MUHAMMAD YOUNIS, DANIELA MILOVIC, FAYEQUA B. MAJID, ANJAN BISWAS, MILIVOJ BELIC

Viewed 50 times

Analytical study of Thirring solitons in spatially inhomogeneous birefringent fibers

Author: RULONG HE, YUHUA QI, QIN ZHOU

Viewed 39 times

Research on laser photoelectric detection performance and SNR model of space target in laser detection system

Author: YANRAN LI, MINGYONG LIU

Viewed 50 times

Effect of different TM modes on the sensitivity of surface plasmon resonance based optical fiber sensor

Author: SAXENA PRAGYA, PRADEEP TEOTIA, R. S. KALER

Viewed 32 times

Fiber optic coupler displacement sensor for detection of glucose concentration in distilled water

Author: M. YASIN, SAMIAN, F. N. AINI

Viewed 37 times

Water vapor concentration detection based on QEPAS sensor

Author: Y. F. MA, Y. HE, J. B. ZHANG, G. YU, X. YU, C. CHEN, R. SUN, J. W. ZHANG

Viewed 31 times

Investigation of interaction of carbon dioxide with ionic liquid filled photonic crystal fiber

Author: SERRA DOĞANATA, SEYHAN COŞKUN, YAVUZ ÖZTÜRK, MELTEM ÇELIKOĞLU

Viewed 42 times


Optoelectronics and Advanced Materials, Rapid Communications

20


H Index

Country [Romania](#)**Subject Area and Category** [Engineering](#)
[Electrical and Electronic Engineering](#)[Materials Science](#)
[Electronic, Optical and Magnetic Materials](#)**Publisher** [Institutul National de Cercetare-Dezvoltare pentru Optoelectronica](#)**Publication type** Journals**ISSN** 18426573**Coverage** 2008-ongoing

Quartiles

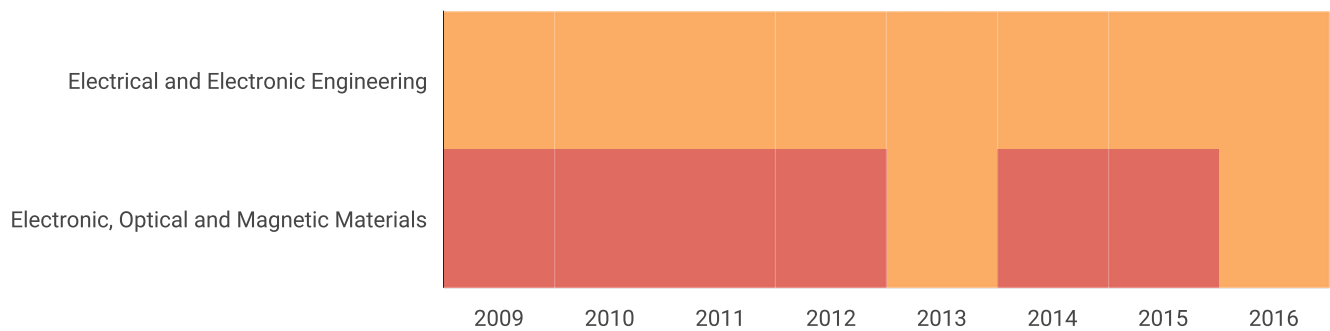







SJR

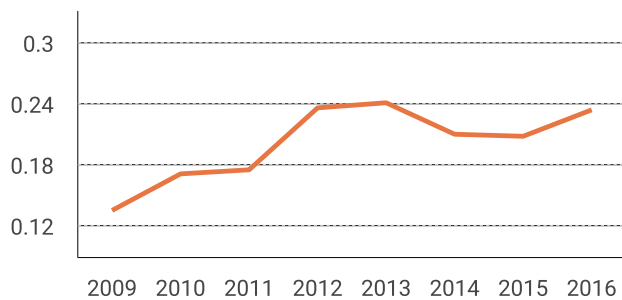

Citations per document

Total Cites

Self-Cites

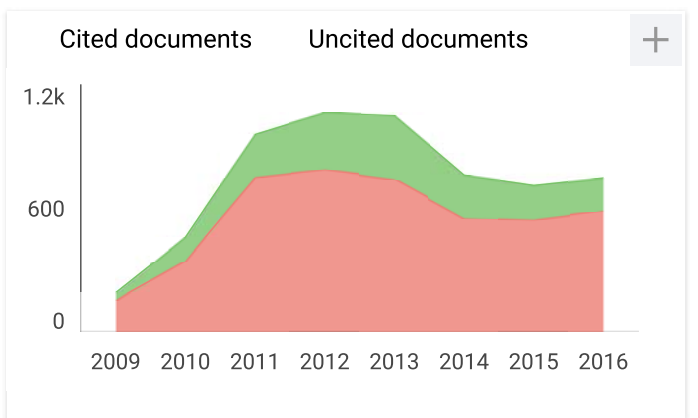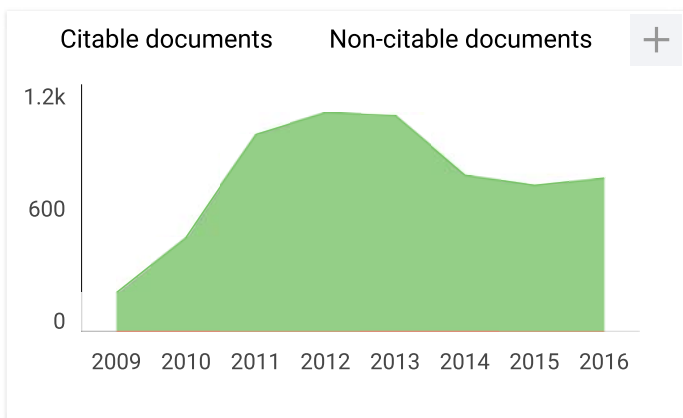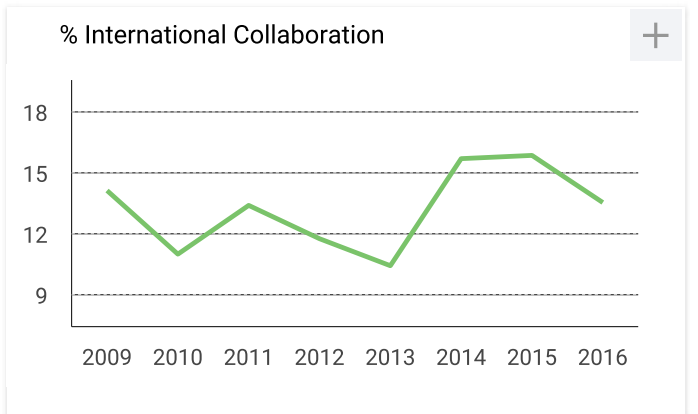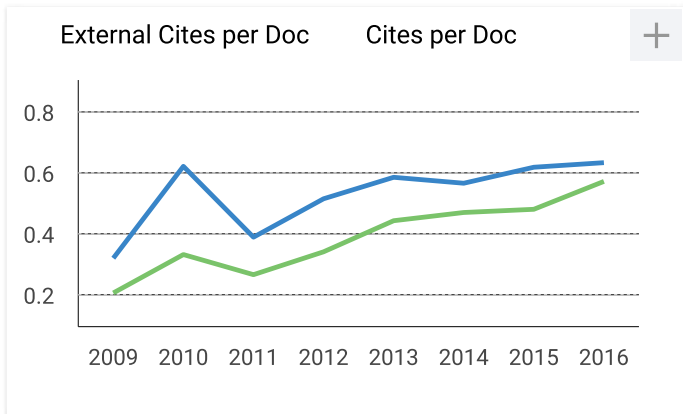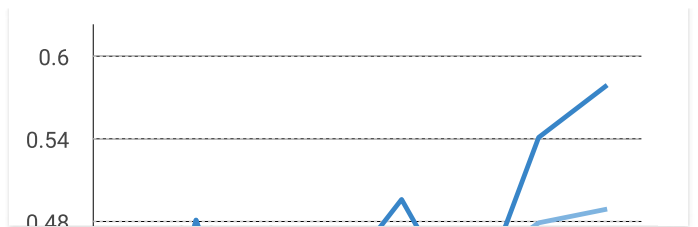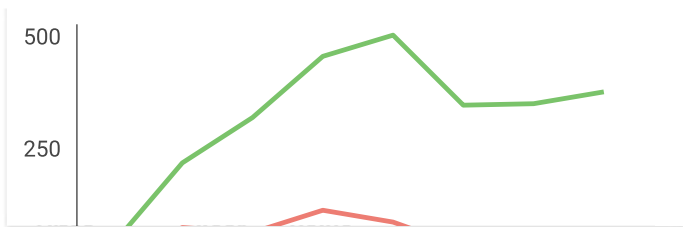

← Show this widget in your own website

Just copy the code below and paste within your html code:

```
<a href="http://www.scimagojr.com
```

Optoelectronics and Advanced Materials, Rapid Communications

Indicator	2009-2016	Value
SJR		0.23
Cites per doc		0.58
Total cites		363

www.scimagojr.com

Developed by:



Powered by:



Follow us on Twitter

Fiber optic coupler displacement sensor for detection of glucose concentration in distilled water

M. YASIN*, SAMIAN, F. N. AINI

Department of Physics, Faculty of Science and Technology, Airlangga University, Surabaya 60115, Indonesia

A simple intensity modulated displacement sensor is demonstrated using a fused coupler as a probe for measuring glucose concentration in distilled water. It uses a plastic optical fiber (POF) based multimode fused coupler as a probe and a flat mirror as a reflector is captured by the same coupler. The light source is a He-Ne red laser (peak wavelength of 633 nm) which is chopped using a mechanical chopper. The reflected optical signal is detected by the silicon photodiode and the electrical signal is then fed into the lock-in amplifier together with the reference signal of the mechanical chopper. The fiber optic probe is first immersed in de-ionized water to measure the output voltage of a 0 % glucose concentration, followed by liquid with glucose concentrations from 5 % to 25 %. It is found that the peak voltage or the collected light intensity linearly related to the glucose concentration. The sensitivity is measured to be around 0.012 mV/(%) when the glucose concentration is varied from 0 to 25%. It is also observe that the slope of the displacement curve increases linearly with the glucose concentration at a rate of 0.0035 mV/(%)².

(Received January 30, 2016; accepted June 9, 2016)

Keywords: Fiber optic glucose sensor, Glucose in distilled water, Coupler probe, Intensity modulation detection

1. Introduction

Fiber optic sensors provides a great chance for developing of a variety of sensors for a wide range of applications [1–4]. A vast range of physical quantities can be sensed optically such as light intensity, vibration, temperature, pressure, calibration of accelerometers, strain, liquid level, pH, chemical analysis, concentration, density, refractive index of liquids etc [5]. Recently, various kinds of optical fiber sensors have been proposed for glucose measurement. For instance, study by non-invasive sensors is reported using polarimetric method to measure the glucose concentration of the aqueous humour of the human eye in vivo [6]. In another work, Yokota et al., [7] have measured glucose concentration of 0.01 g/dl using fiber Faraday rotator as the polarization modulator and or the polarization compensator.

Glucose detection is very important in diabetic patients and an integral part of pancreas with its controlled insulin release. Fiber optic sensors are commonly constructed from plastic multimode optical fibers, which benefit from low optical signal transmission loss, low cost, compact and compatibility with optical fiber technology. In our earlier work, a fiber-optic displacement sensor was proposed for measuring the refractive index of liquid [8]. In this paper a simple, rugged, low cost and very efficient intensity modulated fiber optic glucose sensor is demonstrated to detect the changes in concentration of the liquid. The sensor consists of a light source, a fused coupler fiber optic probe and a silicon detector. A red 633 nm light from He-Ne laser is launched into the coupler and directed to a region where the light interacts with the glucose liquid. This interaction results in a modulation of

optical intensity and the modulated light is collected by the same optical probe and measured by a detection system. The characteristic of the displacement curve of the sensor is investigated for various concentrations of glucose in distilled water.

2. Experimental setup

The schematic diagram of the experimental set-up for sensing various concentrations of glucose in distilled water is shown in Fig. 1. It uses a plastic optical fiber (POF) based multimode fused coupler as a probe and a flat mirror as a reflector to provide the necessary reflection that will be captured by the same coupler. The light source used is a He-Ne red laser (peak wavelength of 633 nm) which is chopped using a mechanical chopper at 210 Hz to avoid the harmonics from the line frequency and reduce the interference of ambient stray light [9]. The reflected optical signal is detected by the silicon photodiode (818 SL, Newport) and the electrical signal is then fed into the lock-in amplifier (SR-510, Stanford Research System) together with the reference signal of the mechanical chopper. The output result from the lock-in amplifier is then connected to a computer through a RS232 port interface and the signals are processed using Delphi software. The flat mirror is fixed on a piezoelectric stage that can be moved with a 0.1 mm resolution.

The output light from the mechanical chopper is launched into port 1 of the fused coupler. The output powers at ports 3 and 4 are divided equally since the coupling ratio of coupler is 50:50. The light is then launched into the glucose solution via port 3 while port 4

of the coupler can be used to monitor the launched light intensity. The reflected light from the mirror is reflected back to enter the same port of the coupler before the collected light intensity is split equally and routed to port 2 as output. The output light is then sent into the silicon photodetector which is connected to the lock-in amplifier for processing. In this experiment, the displacement of the mirror is done in steps of 50 μm . The fiber optic probe was first immersed in de-ionized water to measure the output voltage of a 0 % glucose concentration, followed by liquid with glucose concentrations from 5 % to 25 %. The measurements were carried out for glucose solutions (Merck KGaA Darmstadt, Germany) with concentrations of 2.5, 5.0, 7.5, 10 and 12.5 g per 50 ml of de-ionized water. During the experiment, the error due to this temperature variation is negligible [10] as the temperature is kept constant at 25°C.

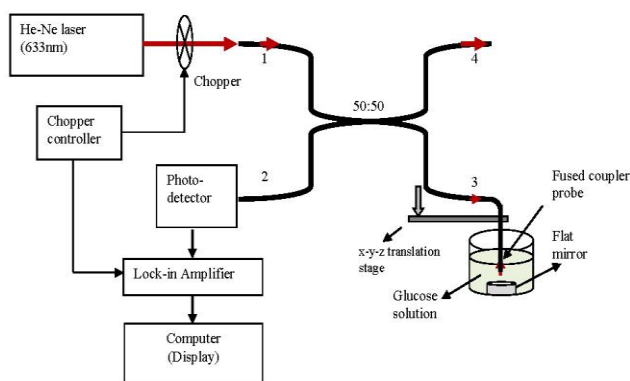


Fig. 1. Experimental setup of FODS for glucose detection using fused coupler

3. Results and discussions

Fig. 2 shows the output voltage characteristic of the proposed sensor against displacement within a range up to 5 mm. The sensor output curve (i.e., light intensity versus distance to flat surface target) indicates only one slope instead of two slopes in the case of bundle fiber [11]. The front slope disappears in this sensor because the transmitting and receiving of light occurs through the same fiber of the coupler. When the gap between the fiber tip and the mirror is zero, the fiber receives the maximum light and thus the measured intensity of the reflected light is the highest at this point as shown in Fig. 2. However, the measured intensity of the reflected light decreases almost linearly with the gap distance especially for close distance target. Theoretically, the distance and the reflected power vary according to the inverse square law, where the output transmission function is given by

$$\frac{P_r}{P_t} = \frac{d^2}{(2x \tan \theta)^2} \quad (1)$$

Where P_r , P_t , d , x , and θ are the reflected power, transmitted power, core diameter, axial displacement and

fiber's acceptance angle, respectively. As shown in Fig. 2, the displacement curve has a slope sensitivity of 0.003 mV/ μm with good linearity of more than 99% within the range of 1.2 mm. The highest resolution of approximately 1 μm is also observed. The stability of the displacement sensor is also investigated and the measurement errors are observed to be less than 0.5% for this sensor.

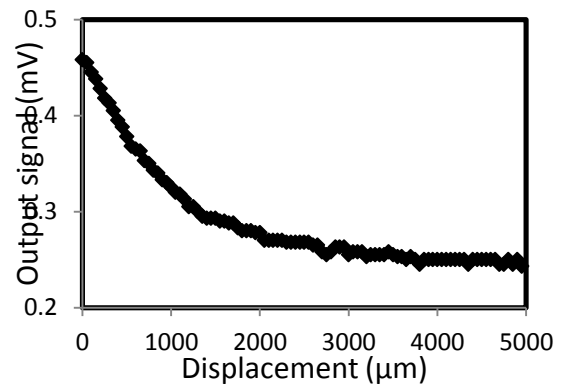


Fig. 2. The Output signal of the sensor as function of displacement

Fig. 3 shows the reflected light intensity versus distance of the reflecting target from the fiber optic probe at various glucose concentrations. In the experiment, the glucose concentration is varied from 0 to 12.5 g per 50 ml of distilled water. As expected, the voltage is highest at zero displacement and the displacements of the receiving fiber away from the target resulted in a reduced output voltage. The output voltage starts to decrease as the receiving fiber is moved away from the target due to the size of the light cone, which increases with the displacement. The power density decreases with increment in the size of the light cone and thus the reflected light intensity, which was measured in term of output voltage, decreases with the displacement. The voltage power at the zero displacement of the curve in Fig. 3 is observed to increase with the concentration of glucose in the de-ionized water. This indicates that the mode coupling with the receiving fiber improves as glucose concentration increases. The variation or modulation of the received light intensity is due to the change of the immersion concentration, which actually changes the emitting and acceptable angle of the fiber probe. The performance of the sensor is summarized in Table 1. The sensitivity can be found from the slope of the curve and obtained at 0.012 mV/% with a good linearity more than 95%. The resolution for the sensor is 2.5% and is sufficiently stable with a standard deviation of 0.016-0.030 mV.

Inset of Fig. 3 shows the variation of peak voltage (maximum voltage at zero displacement) with increasing concentration of glucose. As seen, it is found that the peak voltage increases linearly with the glucose concentration at a rate of 0.012 mV/(%). This is attributed to the refractive index, which proportionally increases with glucose concentration. The increase of refractive index reduces the acceptance angle cone of the fiber-optic probe and the

light intensity received by the receiving fiber due to the reduced acceptance angle cone. The glucose concentration fiber optic has a measured error of less than 0.51% and the

results are repeatable more than six times to get an average.

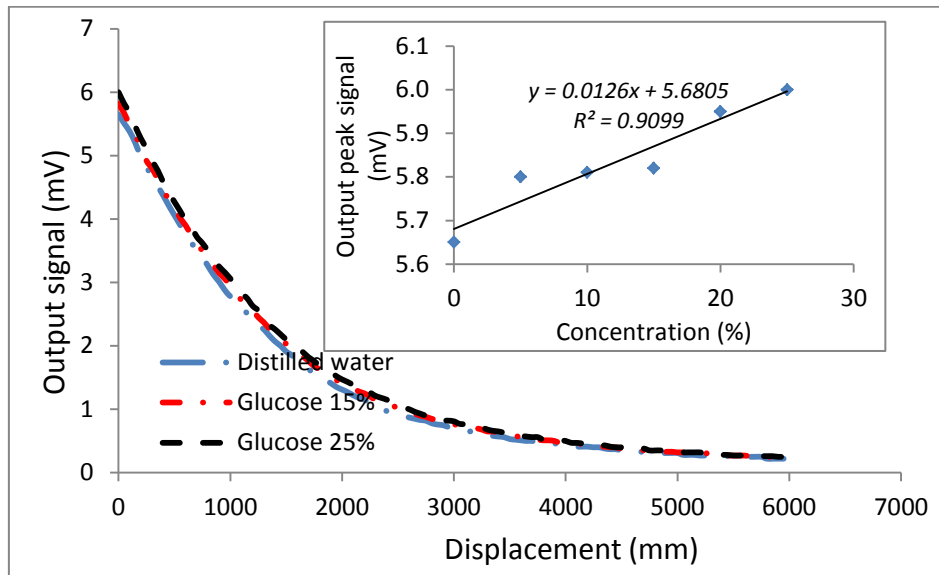


Fig. 3. The output signal as function of the displacement at various glucose solutions. Inset shows the output peak signal versus glucose concentration

Table 1. The performance of FODS for the glucose detection

Parameter	Value
Sensitivity (mV/%)	0.012
Linearity (%)	More than 95
Stability (mV)	0.016-0.030
Resolution (%)	2.5

The performance of the proposed glucose sensor is also investigated based on the slope analysis of the displacement curves. The slope of the displacement curve within the range from 2350 nm to 3000 nm is measured for various glucose concentrations and the result is presented in Fig 4. It is found that the slope increases linearly with the glucose concentration at a rate of $0.0035 \text{ mV}/(\%)^2$. This shows that the peak voltage based analysis is more sensitive than slope based analysis. The resolution is obtained at around 2.5% with the peak voltage measurement approach.

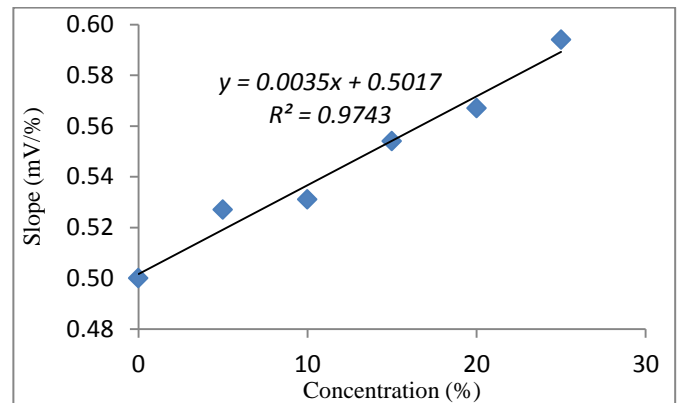


Fig. 4. The slope of displacement curve against the glucose concentration

4. Conclusion

A simple intensity modulated displacement sensor using fused coupler is proposed and investigated for sensing the concentration of glucose in distilled water. For a concentration change of glucose from 0 to 25% in distilled water, the peak light intensity increases linearly with the concentration due to the increased of the refractive index of the liquid. The measured sensitivity and resolution are at around $0.012 \text{ mV}/(\%)$ and 2.5%, respectively. The stability, high sensitivity and simplicity of the sensor make it suitable for chemical, pharmaceutical, biomedical and process control sensing applications.

Acknowledgement

The authors like to express their thanks to Indonesian Directorate General of Higher Education (*DGHE or DIKTI*) through Desentralisasi Research Grant Airlangga University (2014-2015). The authors thank to Prof. Noriah Abidin (Head of Laser Research Group, Universiti Teknologi Malaysia, Malaysia) and Prof. Sulaiman W. Harun (PRC, Univ. of Malaya, Kuala Lumpur, Malaysia) for many discussions and collaboration.

References

- [1] H. A. Rahman, A. I. Che Ani, S. W. Harun, M. Yasin, R. Apsari, H. Ahmad, *Journal of Biomedical Optics*, **17**, 071308-1 (2012).
- [2] S. W. Harun, H. Z. Yang, M. Yasin, H. Ahmad, *Microwave and Optical Technology Letters*, **52**, 373 (2010).
- [3] S. Binu, V. P. Mahadevan Pillai, V. Pradeepkumar, B. B. Padhy, C. S. Joseph, N. Chandrasekaran, *Materials Science and Engineering C*, **29**, 183 (2009).
- [4] M. Yasin, S. W. Harun, W. A. Fawzi, Kusminarto, Karyono, H. Ahmad, *Microwave and Optical Technology Letters*, **51**, 2038 (2009).
- [5] H. A. Rahman, H. R. A. Rahim, S. W. Harun, M. Yasin, R. Apsari, H. Ahmad, W. A. B. Wan Abas., *Optics & Laser Technology*, **45**, 336 (2013).
- [6] G. L. Coté, B. D. Cameron, *J. Biomed. Opt.* **2**, 275 (1997).
- [7] M. Yokota, Y. Sato, I. Yamaguchi, T. Kenmochi, T. Yoshino, *Meas. Sci. Technol.*, **15**, 143 (2004).
- [8] M. Yasin, S.W. Harun, C. F. Tan, S.W. Phang, H. Ahmad, *Microwave and Optical Technology Letters*, **53**, 1935 (2011).
- [9] Anonymous, *Manual Instruction of Model SR510 Lock-In Amplifier*, Stanford Research Systems, Inc., (2003).
- [10] P. Schiebener, J. Straub, J. M. H. Levelt Sengers, J. S. Gallagher., *J. Phys. Chem. Ref. Data*, **19**, 677 (1990).
- [11] M. Yasin, S. W. Harun, Pujiyanto, Z. A. Ghani, H. Ahmad, *Laser Physics*, **20**, 1890 (2010).

*Corresponding author: yasin@fst.unair.ac.id