

Comparison of Frictional Coefficient and Surface Roughness between Three Different Active Self-ligating Brackets An Experimental In Vitro Study

by Meralda R Syahdinda

Submission date: 16-Jul-2020 11:19AM (UTC+0800)

Submission ID: 1358071141

File name: Active_Self-ligating_Brackets_An_Experimental_In_Vitro_Study.pdf (1.21M)

Word count: 3682

Character count: 17938

Comparison of Frictional Coefficient and Surface Roughness between Three Different Active Self-ligating Brackets: An Experimental *In Vitro* Study

Meralda R. Syahdinda, Lucky Lucynda, Ari Triwardhani, Thalca Hamid

Department of Orthodontic, Faculty of Dental Medicine, Universitas Airlangga, Surabaya, Indonesia

ABSTRACT

Aims and Objectives: In orthodontic treatment, the high levels of friction may reduce the effectiveness of the mechanical and decrease tooth movement efficiency. The use of active self-ligating brackets is claimed to possibly reduce friction in orthodontic treatment. The aim of this study was to investigate the three-different active self-ligating orthodontic brackets in frictional coefficient and surface roughness. **Materials and Methods:** This study was true-experiment laboratory with posttest group design to collect the frictional coefficients data from three different active self-ligating brackets. Friction tests were performed on three different active self-ligating brackets—In-Ovation R, Empower, and BioQuick. Each group consists of seven samples of active self-ligating brackets—and stainless steel wire which has been stored in artificial saliva solutions for 14 days. After the friction coefficients of every sample obtained, the bracket clips were separated from the bodies and set on resin acrylic medias. Surface roughness of the bracket clips was evaluated using the atomic force microscope (AFM). A one-way analysis of variance (ANOVA) followed by Scheffe test for comparisons was performed statistically ($P < 0.05$). **Results:** BioQuick and Empower orthodontic brackets produced lower frictional coefficients compared to In-Ovation-R brackets. BioQuick showed least frictional coefficients. Based on the statistical analysis, there was no significant difference of frictional coefficients between Empower and BioQuick. Surface roughness test showed that the clip surface of In-Ovation R produced the maximum roughness, followed by Empower and BioQuick. **Conclusion:** In-Ovation R brackets offered more frictional coefficients and surface roughness than Empower and BioQuick brackets, whereas BioQuick brackets offered the least among all the brackets studied.

Keywords: Active Self-Ligating Bracket, Friction Coefficient, Surface Roughness

Received: 13-2-2020, **Revised:** 12-04-2020, **Accepted:** 08-05-2020, **Published:** XX-XX-XXXX.

INTRODUCTION

Orthodontic treatment using fixed appliances is based on the specific forces that is applied to the teeth through the attachment of brackets.^[1] Extreme friction forces will impede the teeth movement and detract the efficacy of the appliances.^[2] Friction is affected by biological factor—such as saliva, debris, and biodegradation of the appliance's components that has been used—and physical factor as the using of brackets, archwires, and ligations.^[3] The shape, size, and structures of the fixed appliances' components will affect the treatment result.^[4]

The generated forces of bracket and archwire interactions can be measured from its surface roughness. Surface roughness is texture of a superficial area that gives impacts to the object against its environment.^[5] Increased surface roughness can increase frictional forces because it enhances the contact area between the bracket and the archwire.^[6]

Address for correspondence: Dr. Ari Triwardhani,
Department of Orthodontic, Faculty of Dental Medicine, Universitas
Airlangga, Jl Mayjen Prof. Dr. Moestopo 47, Surabaya, Indonesia.
E-mail: ari-t@fkg.unair.ac.id

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

For reprints contact: reprints@medknow.com

How to cite this article: Syahdinda MR, Lucynda L, Triwardhani A, Hamid T. Comparison of frictional coefficient and surface roughness between three different active self-ligating brackets: An experimental *in vitro* study. *J Int Oral Health* 2020;XX:XX-XX.

Access this article online

Quick Response Code:



Website:
www.jioh.org

DOI:
10.4103/jioh.jioh_53_20

Along with the development in orthodontics, many experiments have been done in order to decrease the friction between bracket and archwire, particularly in sliding mechanics such as the invention of orthodontic self-ligating bracket.^[7] The mechanism of self-ligating brackets helps teeth to move freely into the normal positions due to the low friction.^[8]

Therefore, the purpose of this research was to investigate the three-different active self-ligating orthodontic brackets in frictional coefficient and surface roughness.

MATERIALS AND METHODS

Study design

This study was true-experiment laboratory with posttest group design to collect the frictional coefficients data from three different active self-ligating brackets of #14 premolar. Friction tests were performed on three different active self-ligating brackets—In-Ovation R (GAC-Dentsply, USA), Group II of Empower (American Orthodontics, Sheboygan, Wisconsin, United State), and Group III of BioQuick (Forestaden, Pforzheim, Germany). The three-different orthodontic self-ligating brackets were examined by means of 016 × 0.022 inches rectangular stainless steel archwire (American Orthodontics, Sheboygan, Wisconsin, United State).

Sample preparation

Samples were divided into three groups of brackets and a group of archwire. Each group of brackets consists of seven samples, whereas the archwire group consists of four archwires which each has been cut into half to get eight pieces in total. Each group was soaked in 6.5 pH of artificial saliva solution in a glass petri dish. All the four petri dishes then wrapped and stored in 37°C incubators for 14 days. Medias to place the brackets were made from 1.3-cm-diameter resin acrylic with iron nail attached as the hook [Figure 1A]. Brackets were fixated using cyanoacrylate adhesive.

Friction and topography test

Brackets and archwires which had been stored in artificial saliva solution were tested using Universal Testing Machine (AG 500 E, Shimadzu Autograph Japan) [Figure 1B]. Archwires were fixated into the brackets by locking the brackets' slot clips. The nail attached in the resin acrylic media would be hooked into the Universal Testing Machine. The friction tests were done on each sample, in 27°C room temperature and dry environment.

As much as 2 N (newton) force was applied to every orthodontic archwire. A total of 21 results were documented (three types of bracket × seven sample). After the friction coefficient details of every sample obtained, the outer part of the bracket clips was marked and separated from the bodies using disc diamond bur. After that, the parts which have already been marked would set

on other resin acrylic medias, so that the inner part of the clip would face upward. Surface roughness of the bracket clips was evaluated using atomic force microscope (AFM) (Bruker) to obtain the numbers of surface deviation and to evaluate its topography structure [Figure 1C].

AFM has a cantilever and a probe that work as detector which would scan the clip surface in 10 micron areas. From the tests, quantitative data (S_a = average roughness) and qualitative data (2D and 3D picture) were obtained.

Statistical analysis

Analysis of variance was done to examine the difference between groups continued by Scheffe test ($P < 0.05$) or Kruskal–Wallis was done to compare the difference continued by Wilcoxon Mann–Whitney ($P < 0.05$) based on the result of Levene test and Shapiro–Wilk statistical analysis ($P > 0.05$).

RESULTS

Frictional test

In-Ovation R brackets produced higher frictional coefficients than Empower and BioQuick. BioQuick showed least frictional coefficients. Based on the statistical analysis, there was no significant difference of frictional coefficients between Empower and BioQuick.

Table 1 shows the descriptive statistics of the frictional forces for active self-ligating brackets. There was significant difference in coefficient frictional between groups were ($P < 0.05$). Scheffe test that presented in Table 2 showed significant mean frictional value differences between In-Ovation R and BioQuick brackets, as well as In-Ovation R and Empower ($P < 0.05$). Meanwhile, Empower and BioQuick showed no frictional coefficient differences.

Surface roughness test

The quantitative data from the surface roughness tests that had been collected show that the bracket clip surface of In-Ovation R produced the maximum roughness, followed by Empower and BioQuick. The Kruskal–Wallis test was used to compare the average between groups continued by Mann–Whitney test to compare the average of each group.

Table 3 shows significant differences of surface roughness among the three experimental bracket groups. The qualitative data showed the same outcome as the statistic results as seen in Figures 2 and 3.

As seen in Figure 2A, the surface of In-Ovation R clip was dominated by dark brown to black areas, whereas in Figure 2B the surface of Empower clip has less dark areas compared to In-Ovation R clip. The surface of BioQuickclip as seen in Figure 2C was more stable with more yellow areas dominated.

Figure 3A shows the surface of In-Ovation clip. It shows an uneven surface, with mostly jagged areas. In the middle area,

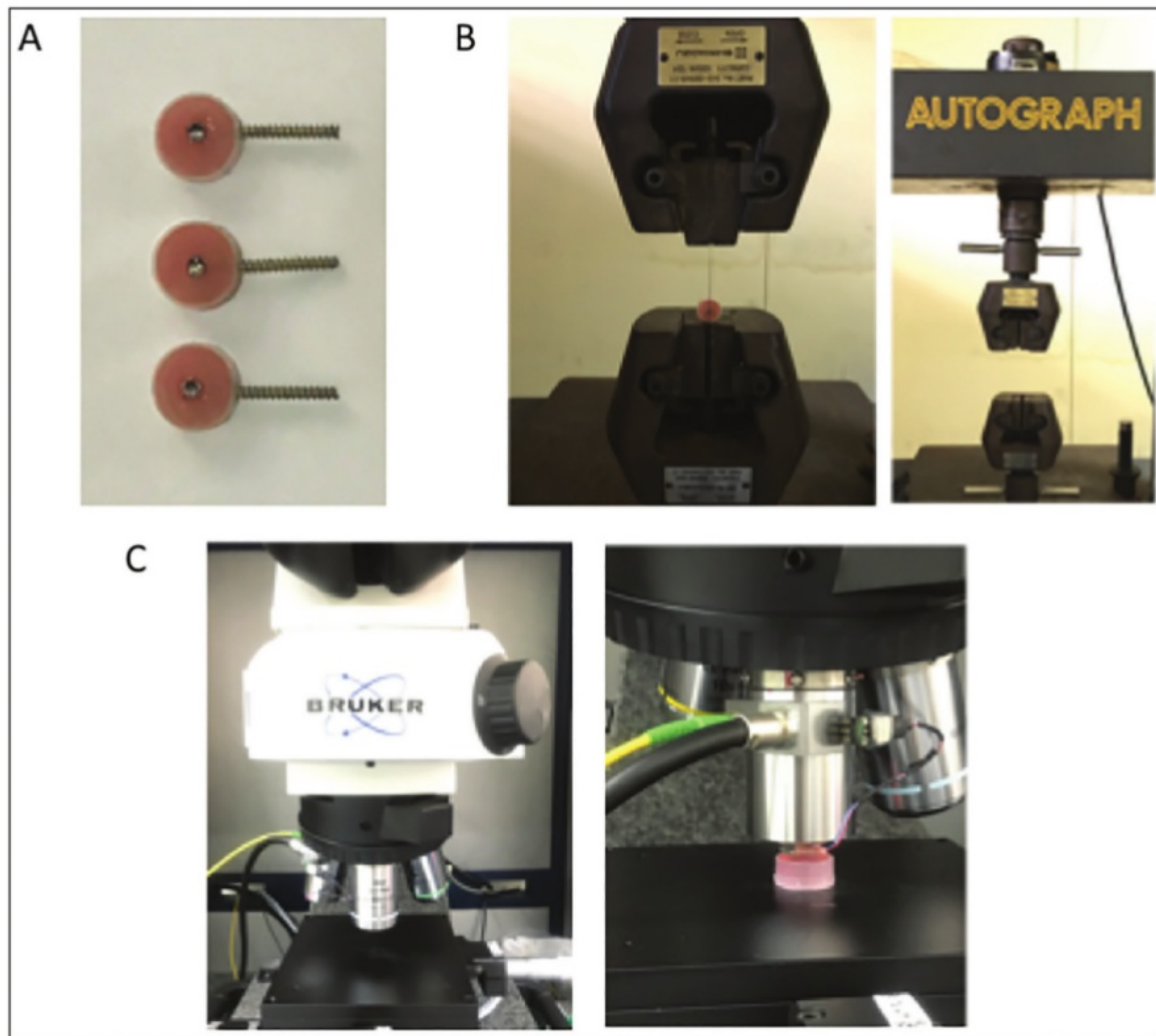


Figure 1: (A) Resin acrylic media for bracket placement. (B) Frictional test using Universal Testing Machine. (C) Surface roughness test using atomic force microscope

Table 1: One-way analysis of variance comparing frictional coefficients in Newton

Bracket	Mean	SD	F Value	P Value
In-Ovation	0.041	0.006	79.947	0.001*
Empower	0.016	0.004		
BioQuick	0.011	0.002		

SD = standard deviation

*Significant at $P < 0.05$

there is a depression which is shown by deep brown color. Figure 3B shows the surface roughness of Empower clip, which is dominated by hollows-like areas. Figure 3C shows BioQuick clip's surface. The surface seems more even compared to In-Ovation and Empower surfaces. The

2D and 3D images from AFM showed that In-Ovation R bracket clip has the highest surface roughness, followed by Empower and BioQuick.

DISCUSSION

According to the previous studies, the teeth movement in sliding mechanics is not a sustainable gliding motions, but series of a very smooth tipping and uprighting motions. During the process of sliding mechanics, the forces that applied to the teeth would cause tipping and rotation.^[9] When the teeth rotate, arch wire will make a contact with the distal edge of the buccal clip/spring clip. The material of the bracket clip would affect the friction value. Material of brackets that produce the highest friction force is β -titanium, followed by nickel-titanium

Table 2: Scheffe test of frictional force comparing interactions between two experimental groups

Scheffe	(I)	(J)	Mean difference (I-J)	Std. error	Sig.	95% Confidence interval	
						Lower bound	Upper bound
	In-Ovation R	BioQuick	0.030000	0.002542	0.001*	0.02322	0.03678
		Empower	0.025000	0.002542	0.001*	0.01822	0.03178
	BioQuick	In-Ovation R	-0.030000	0.002542	0.001*	-0.03678	-0.02322
		Empower	-0.005000	0.002542	0.173	-0.01178	0.00178
	Empower	In-Ovation R	-0.025000	0.002542	0.001*	-0.03178	-0.01822
		BioQuick	0.005000	0.002542	0.173	-0.00178	0.01178

*Significant at $P < 0.05$

(Ni-Ti), cobalt-chromium (Co-Cr), and stainless steel.^[10] Empower and BioQuick clips were made of stainless steel, whereas In-Ovation R clip material were Co-Cr.^[11] Active clip from self-ligating brackets are made of various type of metals with different characteristic and rigidity. The more rigid (or less compressible) the clip material, the higher the friction force produced.^[12] This theory supports the results of this study that is the bracket clip of In-Ovation R, which has Co-Cr material, produced higher friction coefficient than Empower and BioQuick, which have stainless steel as their main material.

In-Ovation R, Empower and BioQuick brackets have spring clips that transfer active forces from archwire to the bracket slot. The ligation mechanism of Empower bracket required its stainless-steel clip to be pulled down to fix the bracket aperture and archwire. The interactive clip is flexible and move in circular motion along with the archwire.^[13] In-Ovation R bracket has agile buckle system which pass by occlusogingival to the edgewise slot. It is a full slot clip coverage that allows interaction between the clip and archwire. In-Ovation R's clip is more rigid than Empower's.^[2] BioQuick bracket has rounded slot edges and contact ribs which can produce minimal friction.^[14]

Aside from its self-ligating mechanism, the main cause of the frictional coefficient differences produced is the geometric design of the brackets. Wider surface brackets will provide lower friction than the narrow ones because archwires can move more freely.^[15] From the previous studies, BioQuick bracket has the widest slot dimension than Empower and In-Ovation R, which is 3,000mm. It supports this study result that BioQuick produced lowest frictional coefficient between the three brackets. Slot of Empower is a little narrower in dimension than BioQuick, 2946mm, whereas for In-Ovation R is 2667mm.^[16] It goes along with this study result that showed In-Ovation R bracket has the highest frictional coefficient.

The result of surface roughness tests in this study is incongruent with the frictional tests result. The previous studies showed that the surface roughness of a material relates to its frictional coefficient.^[17] Surface roughness of the brackets can be affected by its surface structures, such as material, coating, manufacture techniques, and the interaction between bracket and archwire.^[18]

Conclusion

In-Ovation R brackets offered more frictional coefficients and surface roughness than Empower and BioQuick brackets, whereas BioQuick brackets offered the least among all the brackets studied.

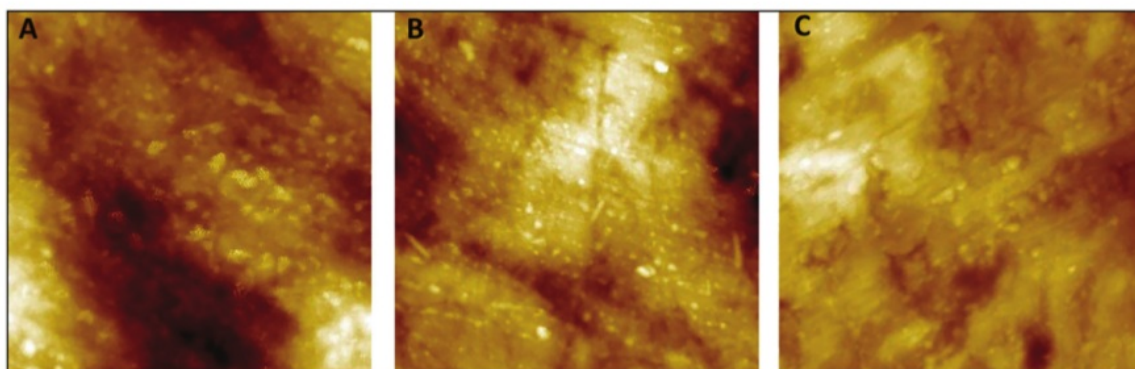
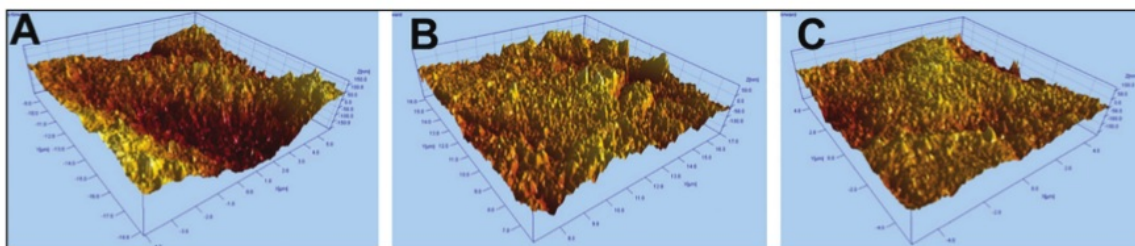
Acknowledgement

The authors wish to thank Faculty of Pharmacy, Universitas Airlangga and Faculty of Material and Metallurgy, Institute Technology Sepuluh Nopember for

Table 3: Comparison of surface roughness among the three experimental bracket groups

Parameters	In-Ovation (N = 7)	Empower (N = 7)	BioQuick (N = 7)	P Value
Range	9.40–11.00	16.40–20.00	15.80–33.00	*
Mean ± std. error	10.29 ± 0.22 ^{ab}	18.23 ± 0.45 ^{bc}	25.94 ± 2.15 ^{bc}	
Median	10.60	18.20	27.60	
Std. deviation	0.59	1.19	5.68	

From Kruskal–Wallis test: *Significant at $P < 0.01$. From Mann–Whitney test: ^aSignificant at $P < 0.05$ in group In-Ovation R and Empower; ^bSignificant at $P < 0.05$ in group In-Ovation R and BioQuick; ^cSignificant at $P < 0.05$ in group Empower and BioQuick

**Figure 2:** 2D surface images of clip brackets: (A) In-Ovation R, (B) empower, and (C) BioQuick using atomic force microscope**Figure 3:** 3D surface images of clip brackets: (A) In-Ovation R, (B) empower, and (C) BioQuick using atomic force microscope

providing support in the conduct of this study and also the staff of the departments for their generous assistance in carrying out the experiments.

Financial support and sponsorship

Nil.

Conflicts of interest

There are no conflicts of interest.

REFERENCES

- Almosa N, Zafar H. Incidence of orthodontic brackets detachment during orthodontic treatment: A systematic review. *Pak J Med Sci* 2018;34:744-50.
- Prashant PS, Nandan H, Gopalakrishnan M. Friction in orthodontics. *J Pharm Bioallied Sci* 2015;7:S334-8.
- Almeida FA, Almeida AP, Amaral FL, Basting RT, Franca FM, Turssi CP. Lubricating conditions: Effects on friction between orthodontic brackets and archwires with different cross-sections. *Dental Press J Orthod* 2019;24:66-72.
- Papageorgiou SN, Keilig L, Hasan I, Jager A, Bourauel C. Effect of material variation on the biomechanical behaviour of orthodontic fixed appliances: A finite element analysis. *Eur J Orthod* 2016;38:300-7.
- Rudge P, Sherriff M, Bister DA. Comparison of roughness parameters and friction coefficients of aesthetic archwires. *Eur J Orthod* 2015;37:49-55.
- Usui T, Iwata T, Miyake S, Otsuka T, Koizumi S, Shirakawa N, et al. Mechanical and frictional properties of aesthetic orthodontic wires obtained by hard chrome carbide plating. *J Dent Sci* 2018;13:151-9.
- Faizee KM, Thomas S, Khrisnaswamy NR. Frictional characteristics of active and passive self-ligation bracket systems: An *in vitro* Study. *J Indian Orthod Soc* 2011;45:154-9.
- Jangde A, Garg A, Virang B, Sahu S. Self ligating brackets from past to present: An update. *IOSR J Dent Med Sci* 2018;17:30-43.
- Ribeiro GL, Jacob HB. Understanding the basic of space closure in orthodontic for a more efficient orthodontic treatment. *Dent Press J Orthod* 2016;21:115-25.
- Kumar D, Dua V, Mangla R, Solanki R, Solanki M, Sharma R. Frictional force released during sliding mechanics in nonconventional elastomers and self-ligation: An *in vitro* comparative study. *Indian J Dent* 2016;7:60-5.
- Franco EM, Valarelli FP, Fernandes JB, Cancado RH, Freitas KM. Comparative study of torque expression among active and passive self-ligating and conventional brackets. *Dental Press J Orthod* 2015;20:68-74.

1	12. Gómez-Gómez S-L, Villarraga-Ossa J-A, Diosa-Peña J-G, Ortiz- Restrepo J-F, Castrillón-Marín R-A, Ardila, CM, <i>et al.</i> Comparison of frictional resistance between passive self-ligating brackets and slide-type low-friction ligature brackets during the alignment and leveling stage. <i>J Clin Exp Dent</i> 2019;11:e593-600.	15. Lee SM, Hwang CJ. A comparative study of frictional force in self-ligating brackets according to the bracket-archwire angulation, bracket material, and wire type. <i>Korean J Orthod</i> 2015;45:13-9.	1
2			2
3			3
4			4
5	13. Francisconi MF, Janson G, Henriques JF, Freitas KM, Francisconi PA. Evaluation of the force generated by gradual deflection of 0.016-inch niti and stainless steel orthodontic wires in self-ligating metallic and esthetic brackets. <i>J Clin Exp Dent</i> 2019;11:e464-9.	16. Thariq VK, Dilip S. Comparison of frictional resistance between interactive self ligating, passive self ligating and conventional orthodontic brackets—an <i>in vitro</i> study. <i>IOSR J Dent Med Sci</i> 2013;10:19-23.	5
6			6
7			7
8			8
9	14. Cappellette M. <i>In vitro</i> comparison of friction generated by various models of self-ligating and conventional brackets while performing retraction with sliding mechanics. <i>Global J Med Res J Dent</i> <i>Otolaryngol</i> 2017;17:1.	17. Kumar A, Khanam A, Ghafoor H. Effects of intraoral aging of arch-wires on frictional forces: An ex vivo study. <i>J Orthod Sci</i> 2016;5:109-16.	9
10			10
11			11
12			12
13			13
14			14
15			15
16			16
17			17
18			18
19			19
20			20
21			21
22			22
23			23
24			24
25			25
26			26
27			27
28			28
29			29
30			30
31			31
32			32
33			33
34			34
35			35
36			36
37			37
38			38
39			39
40			40
41			41
42			42
43			43
44			44
45			45
46			46
47			47
48			48
49			49
50			50
51			51
52			52
53			53
54			54
55			55
56			56

Comparison of Frictional Coefficient and Surface Roughness between Three Different Active Self-ligating Brackets An Experimental In Vitro Study

ORIGINALITY REPORT

12%

SIMILARITY INDEX

8%

INTERNET SOURCES

10%

PUBLICATIONS

6%

STUDENT PAPERS

PRIMARY SOURCES

1	Submitted to Universitas Airlangga Student Paper	4%
2	www.science.gov Internet Source	1%
3	worldwidescience.org Internet Source	1%
4	www.jaypeejournals.com Internet Source	1%
5	synapse.koreamed.org Internet Source	1%
6	www.ijpsonline.com Internet Source	<1%
7	Hasan , Zainab M. Ali , Fakhri A.. "Nugget Mechanical Properties of Combination (Rectangular and Round) Welded and Soldered Stainless Steel Wires", College of Dentistry : Baghdad University, 2014.	<1%

-
- 8 Krishnan, M.. "Comparative evaluation of frictional forces in active and passive self-ligating brackets with various archwire alloys", American Journal of Orthodontics & Dentofacial Orthopedics, 200911
Publication <1%
-
- 9 www.revodontolunesp.com.br
Internet Source <1%
-
- 10 repository-tnmgrmu.ac.in
Internet Source <1%
-
- 11 "ABSTRACTS OF LECTURES AND POSTERS: EUROPEAN ORTHODONTIC SOCIETY, 86th Congress Portoroz, Slovenia 2010, 15-19 June", The European Journal of Orthodontics, 2010
Publication <1%
-
- 12 jacobspublishers.com
Internet Source <1%
-
- 13 Lorenz M. Brauchli, Christiane Senn, Andrea Wichelhaus. "Active and passive self-ligation—a myth?", The Angle Orthodontist, 2011
Publication <1%
-
- 14 www.jehp.net
Internet Source <1%
-
- 15 Agarwal, S.. "Self-ligating brackets", American Journal of Orthodontics & Dentofacial <1%

16

Pandis, N.. "Active or passive self-ligating brackets? A randomized controlled trial of comparative efficiency in resolving maxillary anterior crowding in adolescents", American Journal of Orthodontics & Dentofacial Orthopedics, 201001

Publication

<1%

17

S. Shimbo, N. Matsuda-Inoguchi, T. Watanabe, K. Sakurai, C. Date, A. Nishimura, H. Nakatsuka, H. Saito, K. Arisawa, M. Ikeda. "Dietary intake of tin in Japan, and the effects on intake of canned food and beverage consumption", Food Additives and Contaminants, 2007

Publication

<1%

18

Kahlon, S.. "In-vitro evaluation of frictional resistance with 5 ligation methods and Gianelly-type working wires", American Journal of Orthodontics & Dentofacial Orthopedics, 201007

Publication

<1%

19

Erika Hoyama, Silvana A. Schellini, Mariângela E. A. Marques, Romualdo Rossa, Carlos R. Padovani. "A Comparison of Human and Porcine Acellular Dermal Tissues in the Subcutaneous Space of a Rat Model", Orbit,

<1%

2009

Publication

20

Fariborz Amini, Vahid Rakhshan, Maryam Pousti, Hajir Rahimi, Mahsa Shariati, Bahareh Aghamohamadi. "Variations in surface roughness of seven orthodontic archwires: an SEM-profilometry study", The Korean Journal of Orthodontics, 2012

Publication

<1%

Exclude quotes On

Exclude matches Off

Exclude bibliography On

Comparison of Frictional Coefficient and Surface Roughness between Three Different Active Self-ligating Brackets An Experimental In Vitro Study

GRADEMARK REPORT

FINAL GRADE

/100

GENERAL COMMENTS

Instructor

PAGE 1

PAGE 2

PAGE 3

PAGE 4

PAGE 5

PAGE 6
