A Comparative Study Between Filtered Back Projection (FBP) and Sinogram-Affirmed Iterative (SAFIRE) Reconstructions on HRCT Chest of COPD Patients to Measure the

by Ayub Manggala Putra

ORIGINAL ARTICLE

A Comparative Study Between Filtered Back Projection (FBP) and Sinogram-Affirmed Iterative (SAFIRE) Reconstructions on HRCT Chest of COPD Patients to Measure the Quantity of Emphysema and Lung Volumes

Ayub Manggala Putra[1], Lailatul Muqmiroh[1,2], Budi Prijo Witjaksono[3], Rosy Setiawati[3,4], Amilia Kartikasari[1,2], Pham Minh Thong[5], Vu Dang Luu[5], Cong Tien Nguyen[5], Phan Anh Phuong[5], Le Van Chuyen[5]

[1] Radiologic Imaging Technology Program, Department of Health, Faculty of Vocational Studies, Universitas Airlangga, 60286 Gubeng, Surabaya, Indonesia
[2] Department of Health, Faculty of Vocational Studies, Universitas Airlangga, 60286 Gubeng, Surabaya, Indonesia
[3] Radiodiagnostic Division, Dr. Soetomo General Hospital, 60286 Gubeng, Surabaya, Indonesia
[4] Department of Radiology, Faculty of Medicine, Jl Prof. Moestopo 47, 60131, Surabaya, Indonesia
[5] Radiology Department, Bach Mai Hospital, 100000 Dong Da, Hanoi, Vietnam

ABSTRACT

Introduction: Chest High Resolution Computed Tomography (HRCT) plays a role in determining the emphysema severity levels of COPD patients by measuring the low-attenuation volume (LAV) of the lung parenchyma. **Methods:** This can be used as an alternative to calculate the lung volumes and provide additional information on the pathology that causes both the increase and the decrease of lung volumes. Generally, the reconstruction of raw data in HRCT uses Filtered Back Projection (FBP). Nowadays, reconstruction technology that can be used as an alternative for HRCT is reconstruction iterative (IR) to maximize the diagnosis information and the image quality in a low radiation dose. Sinogram-Affirmed Iterative Reconstruction (SAFIRE) is an iterative reconstruction using noise modelling technique. The research aimed at comparing the use of FBP reconstruction using SAFIRE to measure the quantity emphysema and lung volumes. **Results:** A reconstruction using window lung filter kernel B70f sharp and reconstruction using SAFIRE soft tissue standard I70f sharp were performed to 40 samples. A post-processing, then, was conducted to each of the reconstruction result to measure the quantity of emphysema by displaying the Low Attenuation Volume (LAV%) values and lung volumes (ml). **Conclusion:** The result of the research shows that the use of reconstruction using SAFIRE can affect the measurement result of the quantity of emphysema and lung volumes quantitatively by using a post-processing software when compared to the reconstruction using FBP with the significant values ($p < 0{,}05$).

Keywords: FBP, SAFIRE, HRCT, Iterative Reconstruction, COPD, Emphysema Quantity, Lung volumes

Corresponding Author:
Lailatul Muqmiroh, Sp.Rad (K)
Email: lailatul.muqmiroh@vokasi.unair.ac.id
Tel: +62-031-5033869

INTRODUCTION

Chronic Obstructive Pulmonary Disease (COPD) is a respiratory disease that has become one of the leading causes of death. COPD includes emphysema and chronic bronchitis (1). Based on the previous studies involving 13 Asian countries, the highest prevalence of COPD due to smoking habits is Vietnam, which is 6,7% and the lowest one is Hongkong, which is 3.5% (2). Meanwhile, in Indonesia, the prevalence of COPD is 3,7%. This is closely related to the increase

of smoking habits of people above 15 years old from 34,2% in 2007 to 36,3% (3) in 2013.

As parts of COPD, emphysema can be diagnosed through the CT-Scan examination. High Resolution Computed Tomography (HRCT) Chest can play a role to determine the emphysema severity levels and the distribution of disease patterns by measuring the Low-attenuation areas (LAA) or low-attenuation volume (LAV) on the lung parenchyma (4). HRCT can also be used as an alternative to calculate the lung volumes by using a post-processing software, providing additional information in diagnostic pathology towards the causes of either the increasing or decreasing volumes of the lung (5).

The development of the role of the *Computed Tomography*, especially HRCT *Chest* is aligned with the development of technology aiming at maximizing diagnosis information and image qualities with minimum radiation doses. As a result, in the last decades, algorithm iterative reconstruction method has been developed (6). Sinogram-Affirmed Iterative Reconstruction (SAFIRE) is one of the iterative algorithm reconstruction methods that uses noise modelling technique (7). SAFIRE has 5 (five) levels of iterative power equal to the levels of minimizing the noises that have been produced. According to the image quality, level 5 (five) has the lowest value and displays artefacts although the noises produced are minimum. Meanwhile, level 1 (one) has a value close to the FBP reconstruction and gives little effect on the *noise* reduction (8,9). Consequently, it has the potential to be used on SAFIRE level 2,3 and 4.

Before the iterative algorithm reconstruction was developed, *Filtered Back Projection* (FBP) became the reconstruction method used for CT-Scan images (10). Many studies used it as a reference of HRCT Chest to measure the lung volumes and the quantity of emphysema (4,11,8).

This research aims at comparing FBP to SAFIRE in the measurement of the quantity of emphysema and lung volumes

MATERIALS AND METHODS

Samples
Approved by Radiology Department Bach Mai Hospital, this research was retrospective and the data were obtained from Radiology Center of Bach Mai Hospital, Vietnam. We excluded samples that met the following criteria: 1) COPD Patients with ventilators, 2) Cutis emphysema, 3) Chest trauma, 4) Field Of View (FoV) that does not include the entire lung, 5) Beam hardening artefacts in lung parenchyma.

CT Scan Technique
Data were obtained from patients that had undergone HRCT Chest without contrast using modalities of CT-Scan Siemens SOMATOM Definition EDGE 128 Slice retrospectively for 3 (three) months by using parameters including Care kV semi 120 kV which is recommended for the adult patient also will be optimal to combine with Activated Care Dose 4D, recon slice thickness 1.0 mm. The data were, then, collected and reconstructed by using kernel filter B70f sharp lung window and SAFIRE soft tissue standard l70f sharp level 2,3 and 4 shown in Figure 1.

Each result of the reconstruction was processed by using 3D Pulmo software in SYNGO.VIA Siemens workstation to measure the quantity of emphysema by displaying the Low Attenuation Volume (LAV) with HU values of -950 in percentage (%) and lung volumes by showing

the symbol of vol in milliliter (ml) while visually the software allows masking the area with certain HU and calculating automatically from Dicom formatted images of HRCT Chest. The area with <-950HU which is detected as emphysema is shown in blue while the airway showed in red shown in Figure 2.

Figure 1 : Parameter Setting in FBP B70F Sharp and SAFIRE l70f (level 2,3,4). The data were, then, collected and reconstructed by using kernel filter B70f sharp lung window and SAFIRE soft tissue standard l70f sharp level 2,3 and 4. Various studies using FBP B70F Sharp as a standard filter in Chest HRCT reconstruction because it can increase spatial resolution which is an important aspect in Chest HRCT.

Figure 2 : Measuring the Quantity of Emphysema (LAV%) and Lung volumes. Each result of the reconstruction was processed by using 3D Pulmo software in SYNGO.VIA Siemens workstation to measure the quantity of emphysema by displaying the Low Attenuation Volume (LAV) with HU values of -950 in percentage (%) and lung volumes by showing the symbol of vol in milliliter (ml). The software allows masking the area with certain HU and calculating automatically from Dicom formatted images of HRCT Chest. The area with <-950HU which is detected as emphysema is shown in blue while the airway showed in red.

Statistical Analysis
The normality test used Shapiro-Wilk test. If the data showed normal distribution, it would be analyzed with ANOVA tests. However, if the data did not display normal distribution, it would be analyzed with Wilcoxon test.

The statistical analysis was performed by using SPSS 25.0 (SPSS, Chicago, IL). A p-value of ≤0.05 was used to represent the statistical significance.

RESULTS

40 samples, consisting of 39 (97,5%) males and 1 (2,5%) female, were obtained from December 2018 to February 2019. The average age was 65,4 years old (ranging from 36-81).
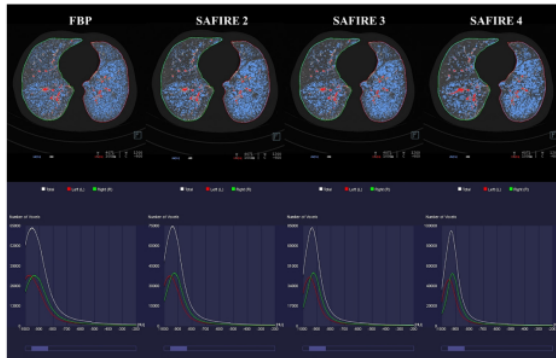
Figure 3 : Shifting in the Histogram of Attenuation Value Distribution. Histogram of attenuation value distribution is one of feature of 3D Pulmo software in SYNGO.VIA that displays a detailed distribution of the Houndsfield Unit (HU) in the voxel of lung area. The implementation of the change of attenuation value distribution can be visually seen from the segmentation result of low attenuation area (LAV) with the threshold of -950HU. There is a shifting of the distribution of attenuation values which move away from the threshold <-950HU, along with the increasing number of the voxel areas in which the distribution of the HU values moving away from the threshold <-950HU

Every reconstruction showed the value distribution of the quantity of emphysema in percentage (LAV%) and lung volumes in millilitre. The distribution of LAV% is shown on Graph 1 and lung volumes is shown on Graph 2.
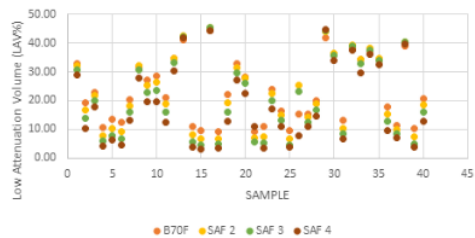
Graph 1 : Low Attenuation Volume (LAV%) Distribution
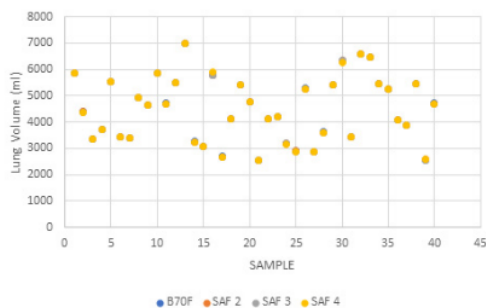
Graph 2 : Lung Volume (ml) Distribution

The significance analysis performed by using Wilcoxon test displays a significant difference on the value of the quantity of emphysema (LAV%) between FBP B70F, SAFIRE l70f level 2,3 and 4 ($p<0.05$). Meanwhile, the significance analysis by using ANOVA showed a significant difference on the value of lung volumes (ml) between FBP B70F, SAFIRE l70f level 2,3 and 4 ($p<0.05$).

DISCUSSION

The Quantity of Emphysema (LAV%)

There are factor affecting the value of the quantity of emphysema (LAV%), one of which is the algorithm reconstruction that was used in HRCT Chest (12). In this research, the value of LAV% from the use of FBP B70F reconstruction and SAFIRE l70f (level 2, 3,4) showed diverse results and, even, significant differences. The result was supported by the research conducted by Choo et al (13) showing the significant differences in the value of the quantity of emphysema (LAV%) or *emphysema index* (EI) between FBP reconstruction on the two types of IR. Baumueller et al (4) also found the similar result showing significant differences in the value of the quantity of emphysema (LAV%) or emphysema index (EI) between FBP reconstructions on one type of IR consisting of various levels.

The consistence of the result of the research confirming the influence of algorithm reconstruction used to produce the value of the quantity of emphysema is based on the theory carried out by Mets et al's (14) research stating that the use of iterative reconstruction on the basis of noise reduction affects the distribution histogram of the attenuation value of lung parenchyma. Areas with low attenuation that is segmented as emphysema has Hounsfield Unit (HU) values below the optimal threshold, -950HU. The noise reduction using iterative reconstruction has a potential to turn the HU values from below the threshold to be equal or above the threshold so that the values will not be segmented as an area that has low attenuation with emphysema (4). SAFIRE as an iterative reconstruction used in this research focused on the noise modelling aimed at reducing noise. It has 5 (five) levels. The higher the level, the stronger the noise reduction (7). Therefore, every level in SAFIRE change the distribution histogram of different attenuation values.

This research used SAFIRE l70f level 2, 3 and 4. As previously mentioned, SAFIRE levels can make changes on the distribution histogram of the different attenuation values due to different noise reduction. The research shows that SAFIRE l70f level 2 has the least significance on FBP B70F. Meanwhile, SAFIRE l70f level 3 and 4, respectively, has the most significance on FBP B70F.

The implementation of the change of attenuation value distribution can be visually seen from the segmentation result of low attenuation area (LAV) with the threshold

of -950HU shown on Figure 3. The samples illustrates that the value of the quantity of emphysema (LAV%) produced on FBP is 33,00%, while on SAFIRE level 2 is 32,30%; SAFIRE level 3 is 30,70%; and SAFIRE level 4 is 28,90%. This indicates that in the histogram there is a shifting of the distribution of attenuation values which move away from the threshold <-950HU, along with the increasing number of the voxel areas in which the distribution of the HU values moving away from the threshold<-950HU.

According to the result of the statistical test Wilcoxon, there was a change in the significance. Not only did the LAV% values decrease, but the LAV% values in each reconstruction also increased. 10 samples (25%) showed the increase or overestimation, while 30 samples (90%) suggested the decrease or underestimation. The range of decreases and increases varied from -0,10 to +15,50 where the differences were obvious. The result of this research is supported by the one conducted by Choo et al (13) who classified the quantity of emphysema and, then, calculated the LAV% values of the results of FBP and IR reconstructions. The research revealed that both groups of LAV% values or emphysema index (EI) decreased when compared with the LAV% values or emphysema index (EI) in FBP reconstruction.

As previously stated, the SAFIRE treatment is an effort to maintain the image quality by reducing the noise. Research conducted by SYang et al (9) showed that there was a noise value reduction in both FBP B70F and SAFIRE l70f reconstructions. The noise occurred due to a fluctuation of CT Number or Hounsfield Unit on the homogenous tissues or materials (15). In a CT Scan device, if one figure with homogenous materials and CT-Number are found in the area, the CT- Number will have various values around the average or mean values. The theory correlated with an attempt to reduce noise on SAFIRE can minimize the fluctuation of HU values in a homogenous tissue. Therefore, there are two possibilities justifying how the underestimation and overestimation on the LAV% values can occur. First, noise reduction can reduce the fluctuation of HU values in the area with normal HU (without emphysema), so some of the areas become homogenous, leading to low HU values (<-950HU) called overestimation. Second, noise reduction can reduce the fluctuation of HU values in the area with low HU (emphysema), so some of the areas become homogenous, leading to normal HU values (>-950HU) called underestimation.

Referred to Goddard Scale (16), severity levels of emphysema were determined by using the values of the quantity of emphysema. Goddard Scale (GS) provides specific evaluation from the percentage of the emphysema quantity values in three lung zones so that the clinical change of the emphysema quantity values, i.e. underestimation or overestimation, can affect the representation result for the Goddard Scale to determine the emphysema severity levels which can be classified into mild, moderate, and severe emphysema.

Lung volumes

Besides the value of the quantity of emphysema (LAV%), this research also discusses the significance values of lung volumes in both FBP and SAFIRE l70f (2,3,4) reconstructions. Research performed by Baumueller et al (4) states that the changes in the lung volumes as a result of segmentation is related to the lung density range which indicates the range of HU values in lung parenchyma by combining the entire volume data. The factor is essential as it affects the differentiation between lung parenchyma and extrapulmonary structures, such as soft tissue, bones and airways. Insignificant change in the lung density range will not affect the segmentation process of lung volumes, while the significant one will change the lung volumes.

According to the statistical analysis, the values of lung volumes in every reconstruction are significantly different. The significance deals not only with the decrease of the values of the lung volumes but also with the increase one in every reconstruction. Compared to the FBP B70F reconstruction, the entire samples of the result of SAFIRE l70f reconstruction show an increase or overestimation in 9 samples (22,5%) and a decrease or underestimation in 31 samples (77,5%).

When correlated with the theory in Baumueller et al's research (4), the changes in lung volumes can be caused by the significant change in lung density range that affects the segmentation process. The implementation of lung density change might not be able to be visually seen through the segmentation result, but it can be assessed through the histogram of the attenuation distribution that shows the shifting in HU values.

Based on the analysis, the change in emphysema quantity values (LAV%) and values of lung volumes (ml) from the use of FBP B70F and SAFIRE l70f reconstructions was caused by the change in attenuation histogram that affect the change in the lung density. Furthermore, the calculation of the value of the quantity of emphysema (LAV%) is quantitatively conducted by using post processing software that has been automatically programmed to process the following formula:

$$LAV\%\text{-}950HU = \frac{\text{low attenuation volume}}{\text{total lung volume}} \times 100\%$$

The formula is used to calculate the LAV% when the threshold is -950HU. Therefore, the formula is relevant if the change of the values of the lung volumes is aligned with the one of values of the quantity of emphysema (LAV%). The analysis result of the formula is different from Baumueller et al's (4) research which showed that there was significant change in the values of the

quantity of emphysema but not in the values of lung volumes. Thus, the analysis in this research can confirm the previous studies according to the theory of formula determining the values of the quantity of emphysema (LAV%) obtained from certain thresholds.

CONCLUSION

The research shows a significant difference ($p<0,05$) on the measurement result of the quantity of emphysema and lung volumes. In other words, the use of SAFIRE reconstruction can affect the measurement result of the quantity of emphysema and lung volumes quantitatively by using a post-processing software when compared to FBP reconstruction.

ACKNOWLEDGEMENT

REFERENCES

1. Zhang WJ, Hubbard Cristinacce PL, Bondesson E, Nordenmark LH, Young SS, Liu YZ, et al. MR Quantitative Equilibrium Signal Mapping: A Reliable Alternative to CT in the Assessment of Emphysema in Patients with Chronic Obstructive Pulmonary Disease. Radiology. 2015;275(2):579–88.
2. Lâm HT, Ekerljung L, Nguy TN, Rönmark E, Larsson K, Lundbäck B. Prevalence of COPD by disease severity in men and women in Northern Vietnam. COPD J Chronic Obstr Pulm Dis. 2014;11(5):575–81.
3. RISKESDAS. Penyakit yang ditularkan melalui udara. Jakarta Badan Penelit dan Pengemb Kesehat Dep Kesehat Republik Indones [Internet]. 2013;(Penyakit Menular):103. Tersedia pada: http://www.academia.edu/download/36235491/Laporan_riskesdas_2010.pdf
4. Baumueller S, Hilty R, Dan T, Nguyen L, Weder W, Alkadhi H, et al. Influence of Sinogram-Affirmed Iterative Reconstruction on Computed Tomography – Based Lung Volumetry and Quantification of Pulmonary Emphysema. 2016;40(1):96–101.
5. Kawakami, Iwano, Hashimoto, Hasegawa, Naganawa. Evaluation of emphysema using three-dimensional computed tomography: association with postoperative complications in lung cancer patients. Nagoya J Med Sci. 2015;77:113–22.
6. Chae IH, Kim Y, Lee SW, Park JE, Shim SS, Lee JH. Standard chest CT using combined automated tube potential selection and iterative reconstruction: Image quality and radiation dose reduction. Clin Imaging. 2014;38(5):641–7.
7. Grant K, Raupach R. SAFIRE : Sinogram Affirmed Iterative Reconstruction. Tech Rep. 2012;1–8.
8. Pavarani A, Martini C, Gafà V, Bini P, Mario S, Sverzellati N. Effect of iterative reconstruction on image quality of low-dose chest computed tomography. Acta Biomed. 2016;87:168–76.
9. Yang WJ, Yan FH, Liu B, Pang ÞLF, Hou L, Zhang H, et al. Can Sinogram-Affirmed Iterative (SAFIRE) Reconstruction Improve Imaging Quality on Low-Dose Lung CT Screening Compared With Traditional Filtered Back. 2013;37(2):301–5.
10. Bushong SC. Radiologic Science for Technologist. Tenth Edit. Radiologic Science for Technologists, 10/e. Elsevier Inc.; 2013.
11. Gallardo-estrella L, Lynch DA, Prokop M, Stinson D, Zach J, Judy PF, et al. Normalizing computed tomography data reconstructed with different filter kernels : effect on emphysema quantification. 2016;478–86.
12. Mets OM, Willemink MJ, Oudkerk M, Prokop M, Jong PA De. The effect of iterative reconstruction on computed tomography assessment of emphysema , air trapping and airway dimensions. 2012;2103–9.
13. Choo JY, Goo JM, Lee CH, Park CM, Park SJ, Shim M-S. Quantitative analysis of emphysema and airway measurements according to iterative reconstruction algorithms : comparison of filtered back projection , adaptive statistical iterative reconstruction and model-based iterative reconstruction. Eur Soc od Radiol. 2014;799–806.
14. Mets OM, Jong PA De, Ginneken B Van, Gietema HA, Lammers JWJ. Quantitative Computed Tomography in COPD : Possibilities and Limitations. 2012;133–45.
15. Seeram E. Computed Tomography: Physical Principles, Clinical Applications, And Quality Control. 3rd ed. Missouri: Elsevier Inc.; 2009.
16. Mohamed YM, Osman NM, Osman AM. Updates In Computed Tomography Assessment Of Emphysema Using Computed Tomography Lung Analysis. Egypt J Bronchol. 2017;11:104–10.

A Comparative Study Between Filtered Back Projection (FBP) and Sinogram-Affirmed Iterative (SAFIRE) Reconstructions on HRCT Chest of COPD Patients to Measure the

8   Geetika Gupta, Sanjai Saxena, Manoj Baranwal, M. Sudhakara Reddy. "In vitro evaluation of bioactive properties of banana sap", Biologia, 2022
Publication

<1 %

9   Anna Winklehner, Christoph Karlo, Gilbert Puippe, Bernhard Schmidt et al. "Raw data-based iterative reconstruction in body CTA: evaluation of radiation dose saving potential", European Radiology, 2011
Publication

<1 %

10   So Won Lee, Yookyung Kim, Sung Shine Shim, Jeong Kyong Lee, Seok Jeong Lee, Yon Ju Ryu, Jung Hyun Chang. "Image quality assessment of ultra low-dose chest CT using sinogram-affirmed iterative reconstruction", European Radiology, 2014
Publication

<1 %

11   academic.oup.com
Internet Source

<1 %

12   Hague, Cameron J., Natasha Krowchuk, Donya Alhassan, Kevin Ho, Jonathon Leipsic, Don D. Sin, John R. Mayo, and Harvey O. Coxson. "Qualitative and Quantitative Assessment of Smoking-related Lung Disease : Effect of Iterative Reconstruction on Low-dose Computed Tomographic Examinations", Journal of Thoracic Imaging, 2014.

<1 %

Publication

13 Medical Radiology, 2016.
Publication

<1%

14 MeiLan K. Han, Ella A. Kazerooni, David A. Lynch, Lyrica X. Liu et al. "Chronic Obstructive Pulmonary Disease Exacerbations in the COPDGene Study: Associated Radiologic Phenotypes", Radiology, 2011
Publication

<1%

15 Nove E. Variant Anna, Dessy Dessy Harisanty, Dyah Puspitasari Srirahayu, Endang Endang Fitriyah Mannan et al. "Developing Information Services for Visually-Impaired Students in Indonesia", International Journal of Engineering & Technology, 2018
Publication

<1%

16 Stephan Baumueller, Regina Hilty, Thi Dan Linh Nguyen, Walter Weder, Hatem Alkadhi, Thomas Frauenfelder. "Influence of Sinogram-Affirmed Iterative Reconstruction on Computed Tomography–Based Lung Volumetry and Quantification of Pulmonary Emphysema", Journal of Computer Assisted Tomography, 2016
Publication

<1%

17 tel.archives-ouvertes.fr
Internet Source

<1%

18 www.nepalmediciti.com
Internet Source

<1 %

19 Young Jun Cho, U. Joseph Schoepf, Justin R.
Silverman, Aleksander W. Krazinski et al.
"Iterative Image Reconstruction Techniques",
Journal of Thoracic Imaging, 2014
Publication

<1 %

Exclude quotes	On	Exclude matches	Off
Exclude bibliography	On		

A Comparative Study Between Filtered Back Projection (FBP) and Sinogram-Affirmed Iterative (SAFIRE) Reconstructions on HRCT Chest of COPD Patients to Measure the

FINAL GRADE

/100

GENERAL COMMENTS

Instructor

PAGE 1

PAGE 2

PAGE 3

PAGE 4

PAGE 5