

The Difference of Plasma Prothrombin Time Value in the Production of Adsorbed Plasma Using Various Concentrations of Barium Sulphate in Dr. Soetomo General Hospital, Surabaya, Indonesia

Putu Devi Oktapiani Putri¹, Paulus Budiono Notopuro²

¹Resident, Clinical Pathology Specialization Program, Department of Clinical Pathology, Faculty of Medicine, Universitas Airlangga, Dr. Soetomo General Hospital, Surabaya, Indonesia, ²Lecturer, Department of Clinical Pathology, Faculty of Medicine, Universitas Airlangga, Dr. Soetomo General Hospital, Surabaya, Indonesia

Abstract

Detection of a factor deficiency in the case of coagulation prolongation is very important, in this case a factor deficient plasma is required. This research provides a simpler method to produce factor deficient plasma, using barium sulphate as an adsorbent with Prothrombin Time (PT) of more than 60 seconds as a target. The aim of this study is to analyze the difference of PT value in various concentrations of barium sulphate. Pooled normal plasma (PNP) was made from citrated blood and basic PT value was measured. Nine plain tubes were prepared with 1 mL of PNP for each tube. Barium sulphate 200-1000 mg/ml plasma was then added to each tube. Finally, PT value of each tube was measured. The presence of barium sulphate <800 mg/ml plasma made no significant changes in PT. Conversely, the presence of ≥ 800 mg/ml plasma increased PT more than 5 times compared to normal PT. Adsorbed plasma lack vitamin K dependent factors because barium sulphate binds to α -polypeptide, and removes all vitamin K dependent factors. The barium sulphate concentration used to make adsorbed plasma in this research was different with previous research. It was found that barium sulphate with ≥ 800 mg/ml plasma can significantly change the PT value, and effectively reach the PT target of adsorbed plasma as a basic reagent for substitution study. In conclusion, different concentrations of barium sulphate used resulted in different PT values. Optimal concentration of barium sulphate to make adsorbed plasma was ≥ 800 mg/ml plasma.

Keywords: *Adsorbed plasma, barium sulphate, plasma prothrombin time.*

Introduction

Prothrombin Time (PT) and Activated Partial Thromboplastin Time (APTT) examinations are routine tests performed to evaluate coagulation function. There are more than 40,000 PPT and APTT examinations at RSUD Dr. Soetomo per year with results that extend by 28%^{1,2}. In order to determine whether the coagulation abnormality is caused by a lack of coagulation factors or

the presence of an inhibitor, a mixing test with normal pooled plasma can be performed. If a coagulation factor deficiency is found, a substitution test can be performed to identify the deficient coagulation factor^{3,4,5}.

Currently, several coagulation factor examinations are available, including the examination of VIII factor and IX factor. Both of these tests can provide information on levels of VIII factor and IX factor; however, these tests are quite expensive and cannot be performed in standard laboratories. The substitution test is a promising alternative as a method of examining coagulation factors. To perform a substitution test, two types of plasma are

Corresponding author:

Putu Devi Oktapiani Putri

Email: devi.oktapiani92@gmail.com

required, namely aged plasma and adsorbed plasma. The availability of these two types of plasma considerably supports the diagnosis of a coagulation disorder, even in a standard laboratory^{6,7,8}.

Preparation of adsorbed plasma requires a standard method so that the adsorbed plasma obtained can be used in the substitution test. In order to produce adsorbed plasma, citrated blood plasma can be mixed with barium sulphate to achieve a predetermined PT value⁹. This research examines the concentrations of barium sulphate that can be used for the manufacture of adsorbed plasma with citrated blood plasma.

Method

This research was conducted using cross-sectional analysis. The samples of this study were collected from veins of Clinical Pathology Resident, Faculty of Medicine, Universitas Airlangga - Dr. Soetomo General Hospital, Surabaya, Indonesia. Random sampling was done until 20 samples were obtained. This research was conducted in the Clinical Pathology Laboratory, Integrated Diagnostic Center Building, Dr. Soetomo General Hospital, Surabaya, Indonesia.

The inclusion criteria were samples from Dr. Soetomo General Hospital, Surabaya, Indonesia which were accommodated in citrate anticoagulant tubes with volume in accordance with the minimum limit of citrate tube filling (2.7 mL). Exclusion criteria were samples with insufficient volume, clotted blood samples, icteric, lipemic, or hemolyzed samples. Independent T-test was performed to analyze the effect of difference of barium sulphate on PPT values. p value <0.05 was considered statistically significant. Data was analyzed using MS excel and SPSS software.

Results and Discussion

The preparation of adsorbed plasma in this study used several variations of barium sulphate concentration. An increase in the concentration of barium sulphate can affect the PT plasma value produced. A very sharp increase in the value of PT was found in the plasma with 900 mg/mL of barium sulphate. With barium sulphate concentration of 1000 mg, the PT value that appeared on the device was *no coagulation*. In this case, the upper limit of the PT value that could be detected by the device was used, namely 130 seconds (Figure 1).

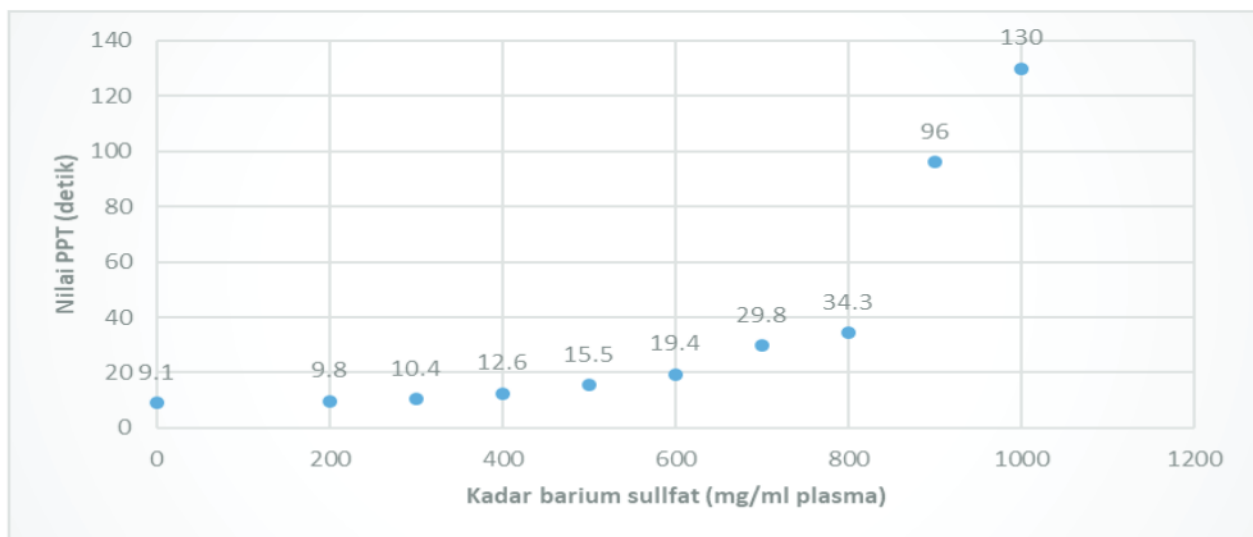


Figure 1. The value of PT in the preparation of adsorbed plasma with various concentrations of barium sulphate.

In this research, several cut-offs of barium sulphate concentrations were chosen to observe how much change in the value of PT would occur when higher concentrations of barium sulphate were used or vice versa. In Table 1, it can be seen that there are 3 cut-offs, namely 600 mg/mL of plasma, 700 mg/mL of plasma, and 800 mg/mL of plasma. A difference test

was performed on each cut-off mean value of PT that could be achieved. In the use of barium sulphate <600 mg/mL of plasma, the mean value of PT was only 11.48 seconds with p value of 0.49, which was not statistically significant. When barium sulphate was used at 800 mg/mL of plasma or above, the PT value was statistically significant reaching 86.77 seconds.

Table 1. The Difference of PT Values with Barium Sulphate Concentration Grouped based on Cutoffs.

Concentration of Barium Sulphate (mg/mL of plasma)	Mean Value of PT (seconds)	p Value
<600 ≥600	11.48 61.90	0.49
<700 ≥700	13.54 72.52	0.29
<800 ≥800	15.23 86.77	0.03

The use of barium sulphate in the preparation of adsorbed plasma has been investigated for decades. Hydrophobic materials such as barium sulphate and aluminum hydroxide can absorb certain coagulation factors (especially II, VII, IX, and X factors) when added to plasma¹⁰. Other studies have shown that the use of aluminum hydroxide can reduce the activity of II, VII, IX, and X factors. Increasing the concentration of aluminum hydroxide used will further reduce the activity of these coagulation factors¹¹. Barium sulphate and plasma citrate was used in this research for the preparation of adsorbed plasma. The greater the concentration of barium sulphate used, the higher the PPT value. This suggests the possibility that the coagulation factors involved in the extrinsic coagulation pathway experience decreased activity.

Vitamin K-dependent coagulation factors have one special feature, which is the fact that they have the same polypeptide structure. In Nelsestuen and Suttie's research, it was found that there was a structure called

α peptide in prothrombin. This structure disappears after adsorption process. This α peptide is a vitamin K dependent structure, and is present in all vitamin K dependent proteins¹².

Adsorption process caused a decrease in the activity of II, VII, IX, and X factors. This study used aluminum hydroxide in gel form as an adsorbent. Each factor showed a different decrease in activity after the adsorption process. This was also influenced by differences in temperature and pH¹¹.

A literature stated that the concentration of barium sulphate used for the preparation of adsorbed plasma is 100 mg/mL of plasma. A different literature stated that 33 grams of barium sulphate is mixed with 150 mL of plasma, to which a buffer solution has been added, then stirred at room temperature for 30 minutes. In this study, the use of barium sulphate below 600 mg/mL of plasma did not significantly increase the PT value. The use of barium sulphate at concentration of 600 mg/mL plasma

produced plasma with PT value of 19.4 seconds (Figure 1). There are several variations in the target value of PT in the preparation of adsorbed plasma, namely 2½ times the normal PT value, or PT >60 seconds¹³. If the upper limit of normal PT value is 13 seconds, then the use of barium sulphate with concentration of 800 mg/mL of plasma would succeed in achieving the minimum target value of PPT, namely 32.5 seconds.

Several cut-offs were selected to determine the appropriate minimum concentration of barium sulphate in the preparation of adsorbed plasma. Based on the PT values achieved with the use of different concentrations of barium sulphate (Figure 1), several cutoffs for barium sulphate concentrations were taken as a reference to achieve the targeted PT value. Using the most minimum concentration of barium sulphate with the most effective result is very important for the efficiency of materials and processing time.

Table 1 shows some of the cutoffs that can be considered as minimal concentrations that can be used for the preparation of barium sulphate. If a lower barium sulphate concentration could achieve the targeted PT value, it would certainly increase the efficiency and effectiveness of the process in making adsorbed plasma. Barium sulphate levels <800 mg did not reach the targeted PT value (Figure 1), and statistically also did not provide a significant difference in PT values (Table 1). Barium sulphate concentration of ≥800 mg/mL of plasma resulted in the most statistically significant p value (p 0.03) with a PPT value that reached 34.3 seconds.

Conclusion

The use of barium sulphate with different concentrations produce plasma with different PT values. Higher levels of barium sulphate increase the plasma PPT value, however the increase is non-linear. Barium sulphate with concentration of ≥800 mg/mL is the most optimal for the preparation of adsorbed plasma as a basic reagent for substitution tests.

Conflict of Interest: The author declare that they have no conflict of interest.

Source of Funding: None.

Acknowledgements: We thank Rr. Putri Amaristya Purwono and Arif Nur Muhammad Ansori for editing the manuscript.

Ethical Approval: The research ethic has been approved by the Ethics Committee of the Faculty of Medicine, Universitas Airlangga, Surabaya, Indonesia.

References

1. Hernaningsih Y, Akualing JS. The effects of hemolysis on plasma prothrombin time and activated partial thromboplastin time tests using photo-optical method. *Medicine*. 2017; 96: 76-79.
2. Hernaningsih Y, Butarbutar TV. The effects of plasma prothrombin time and activated partial thromboplastin time based on different instruments and methods. *J Clin Diagn Res*. 2019; 13: 21-25.
3. Laga AC, Cheves TA, Sweeney JD. The effect of specimen hemolysis on coagulation test results. *Am J Clin Pathol*. 2006; 126: 748-755.
4. Goswami B, Singh B, Chawla R, Gupta VK, Mallika V. Turnaround time (TAT) as a benchmark of laboratory performance. *Indian J Clin Biochem*. 2010; 25: 376-379.
5. Goswami B, Singh B, Chawla R, Mallika V. Evaluation of errors in a clinical laboratory: A one-year experience. *Clin Chem Lab Med*. 2010; 48: 63-66.
6. Dahlbäck B. Pro- and anticoagulant properties of factor V in pathogenesis of thrombosis and bleeding disorders. *Int J Lab Hematol*. 2016; 38: 4-11.
7. Petrillo T, Ayombil F, Van't Veer C, Camire RM. Regulation of factor V and factor V-short by TFPIα: Relationship between B-domain proteolysis and binding. *J Biol Chem*. 2020; 296: 100234.
8. Raditya PPR, Ansori ANM, Notopuro PB. Immune-related pancytopenia: A rare case report in Surabaya, Indonesia. *Biochem Cell Arch*. 2021; 21: 881-884.
9. Cheng Y, Liu J, Su Y, Zhao H, Zhao Y, Wen M, Lu S, Zhang W, Wu J. Clinical impact of coagulation and fibrinolysis markers for predicting postoperative venous thromboembolism in total

- joint arthroplasty patients. *Clin Appl Thromb Hemost.* 2019; 25: 1076029619877458.
10. Sultan A. Five-minute preparation of platelet-poor plasma for routine coagulation testing. *East Mediterr Heal J.* 2010; 16: 233-236.
 11. Swart AC, Klaassen BH, Bloys-van Treslong-de, Hemker HC. The adsorption of blood coagulation factors II, VII, IX and X from human plasma to aluminium hydroxide. *Thromb Diath Haemorrh.* 1972; 27: 490-501.
 12. Nelsestuen GL, Suttie JW. The mode of action of vitamin K. Isolation of a peptide containing the vitamin K-dependent portion of prothrombin. *Proc Natl Acad Sci U S A.* 1973; 70: 3366-70.
 13. Vincent LM, Tran S, Livaja R, Bensen TA, Milewicz DM and Dahlbäck B. Coagulation factor V(A2440G) causes east Texas bleeding disorder via TFPI α . *J Clin Invest.* 2013; 123: 3777-87.